

Sample Name :Somatostatin
 Cat. No. :RP10226
 Lot. No. : PE0181601

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

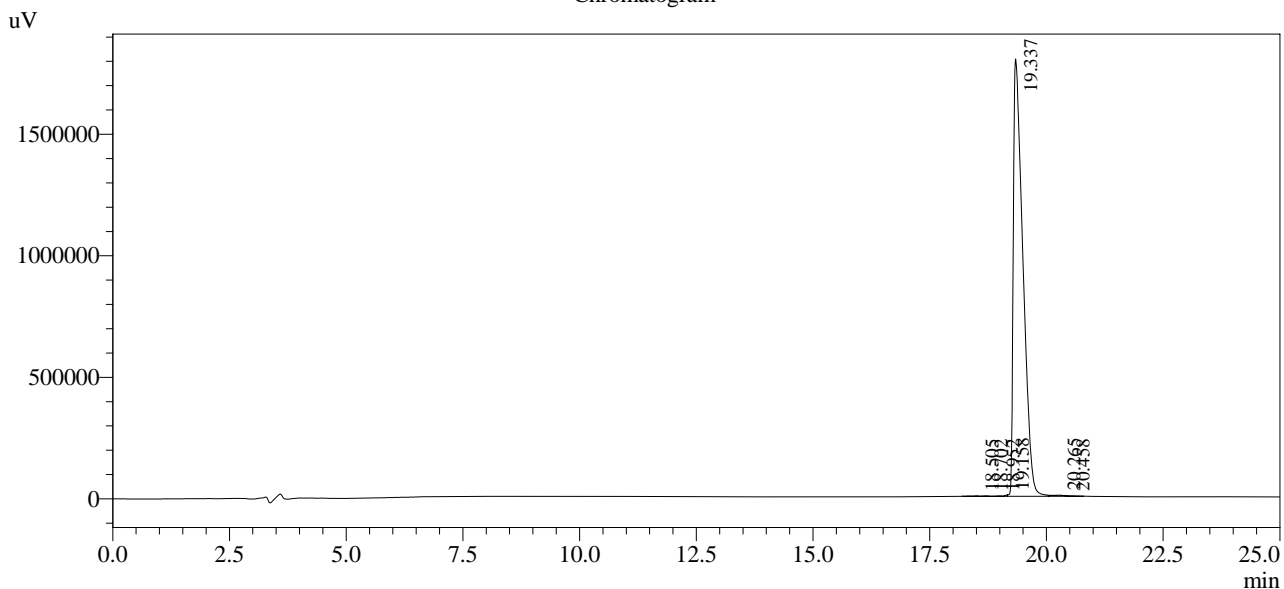

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.505	21368	1672	0.082
2	18.702	12072	1517	0.047
3	18.952	9215	1208	0.036
4	19.158	26539	6139	0.102
5	19.337	25741461	1800098	99.258
6	20.265	93522	4964	0.361
7	20.458	29694	2031	0.114
Total		25933870	1817629	100.000