

Sample Name : Osteogenic Growth Peptide, OGP
 Cat. No. : RP20311
 Lot. No. : PE1091601

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

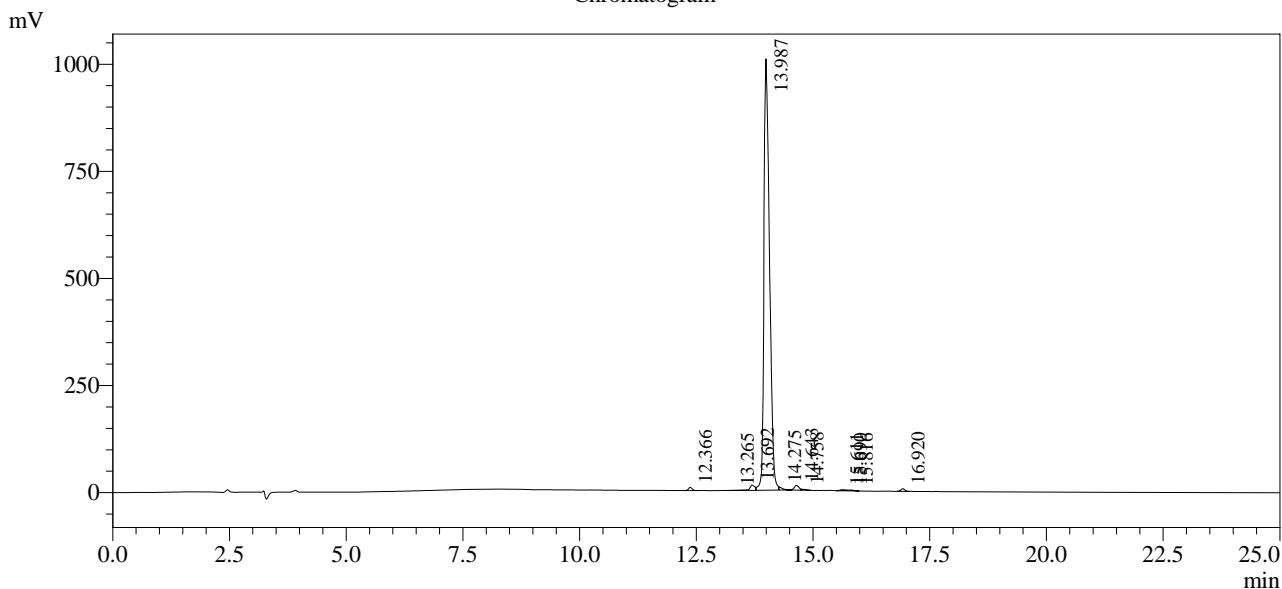

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.366	38766	7248	0.446
2	13.265	6952	1024	0.080
3	13.692	90562	12349	1.043
4	13.987	8349977	1007036	96.166
5	14.275	35421	7145	0.408
6	14.643	75440	10966	0.869
7	14.758	12258	2194	0.141
8	15.611	11905	2315	0.137
9	15.690	13832	2240	0.159
10	15.816	12984	2017	0.150
11	16.920	34814	6271	0.401
Total		8682910	1060804	100.000