

Sample Name : Substance P
 Cat No. : RP10178
 Lot No. : PE0121604

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
39.00	Pumps	Pump B Conc.	5
39.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

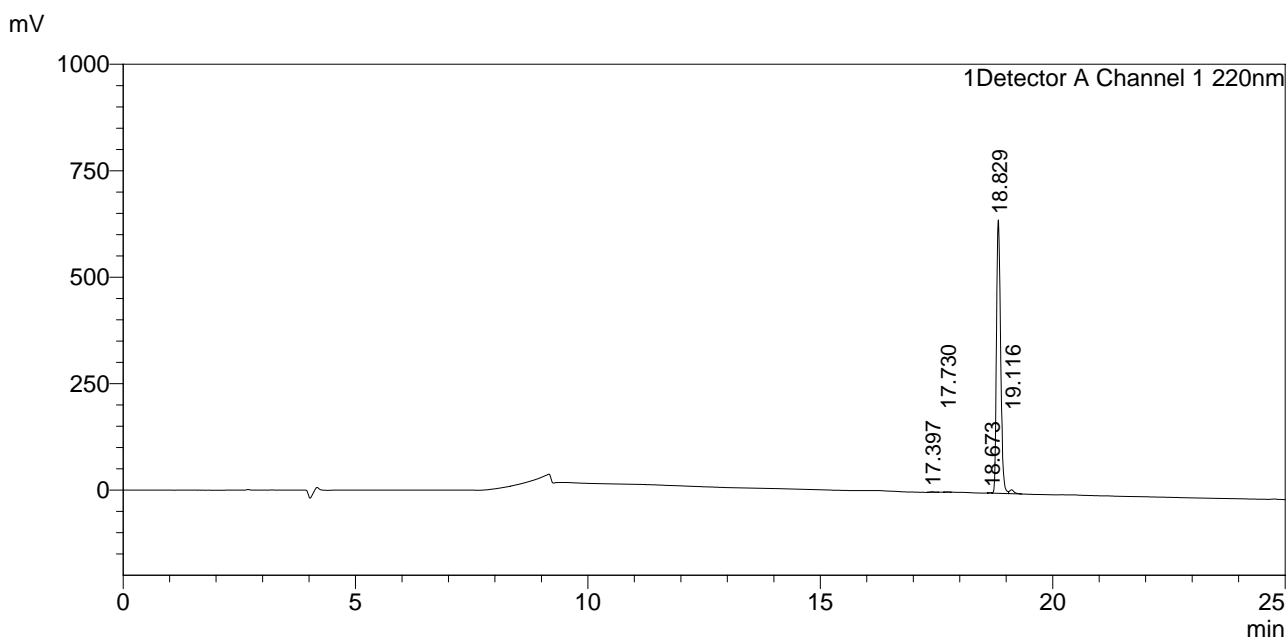

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.397	7464	1265	0.183
2	17.730	2807	552	0.069
3	18.673	4515	1055	0.111
4	18.829	4004878	641120	98.136
5	19.116	61291	9210	1.502
Total		4080955	653202	100.000