

Sample Name : EGFRvIII peptide (PEPvIII)
 Cat No. : RP20356
 Lot No. : PE8001604

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
39.00	Pumps	Pump B Conc.	5
39.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

mV

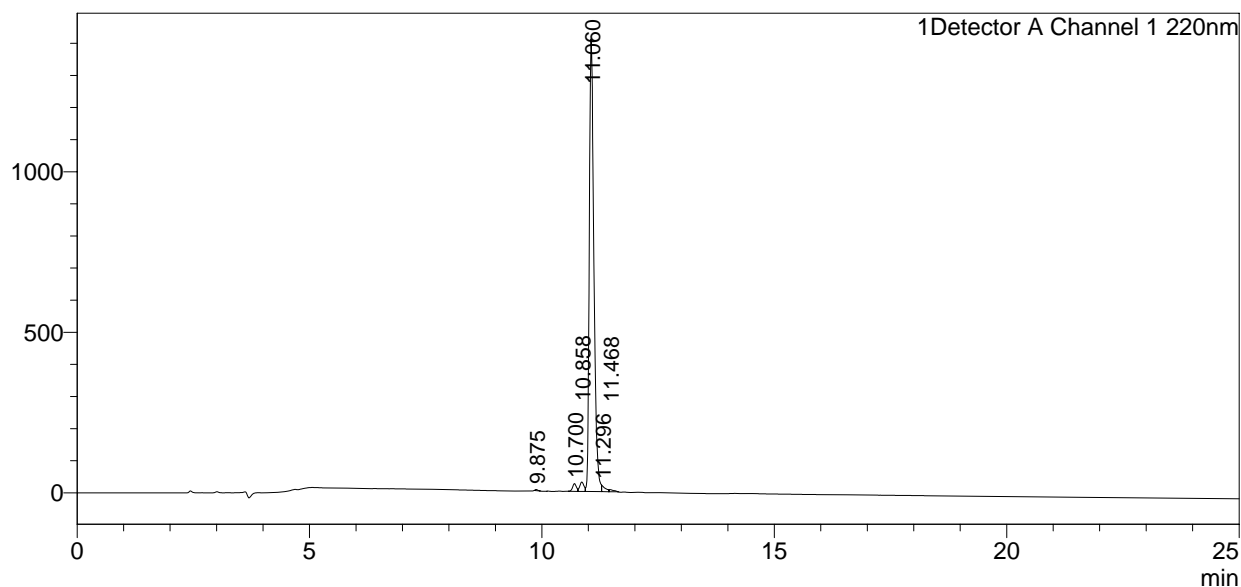

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.875	12511	3332	0.123
2	10.700	139503	24244	1.373
3	10.858	183150	29320	1.803
4	11.060	9673775	1409906	95.230
5	11.296	104609	19538	1.030
6	11.468	44795	6479	0.441
Total		10158344	1492820	100.000