

Sample Name : InsB 9-23
 Cat. No. : RP20391
 Lot. No. : PE6611603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

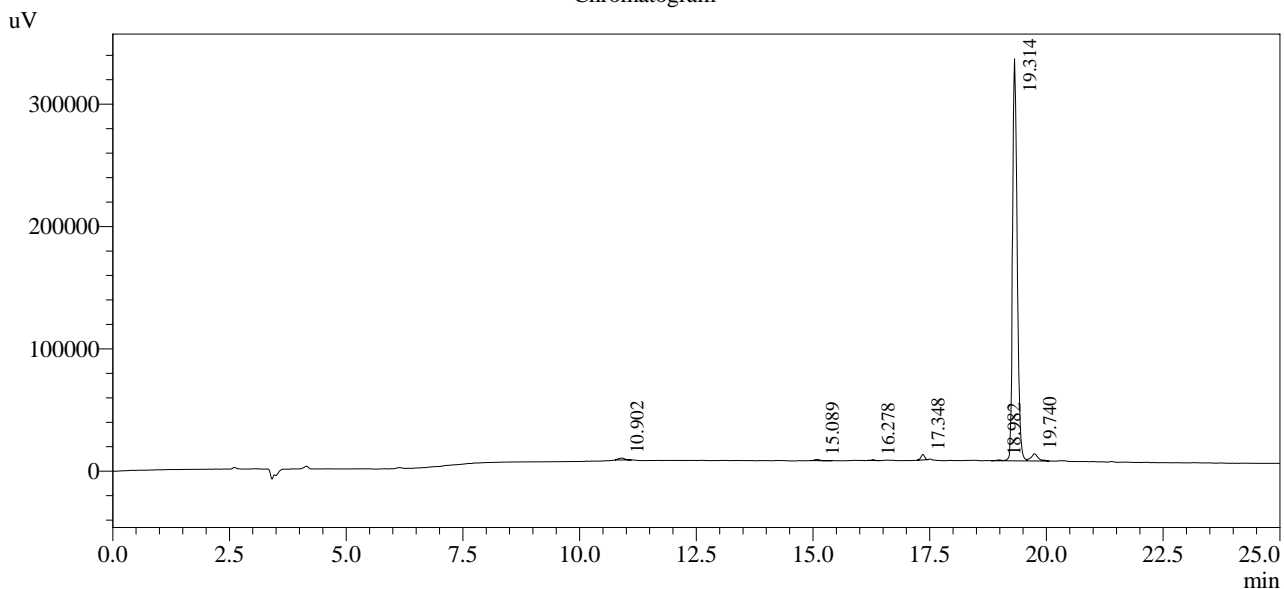

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.902	14195	1538	0.594
2	15.089	6795	984	0.284
3	16.278	2875	643	0.120
4	17.348	24550	4475	1.027
5	18.982	5470	694	0.229
6	19.314	2274013	328673	95.126
7	19.740	62637	5906	2.620
Total		2390535	342914	100.000