

Sample Name :LCMV gp33a-41
 Cat. No. :RP20257
 Lot. No. :PE9041603

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

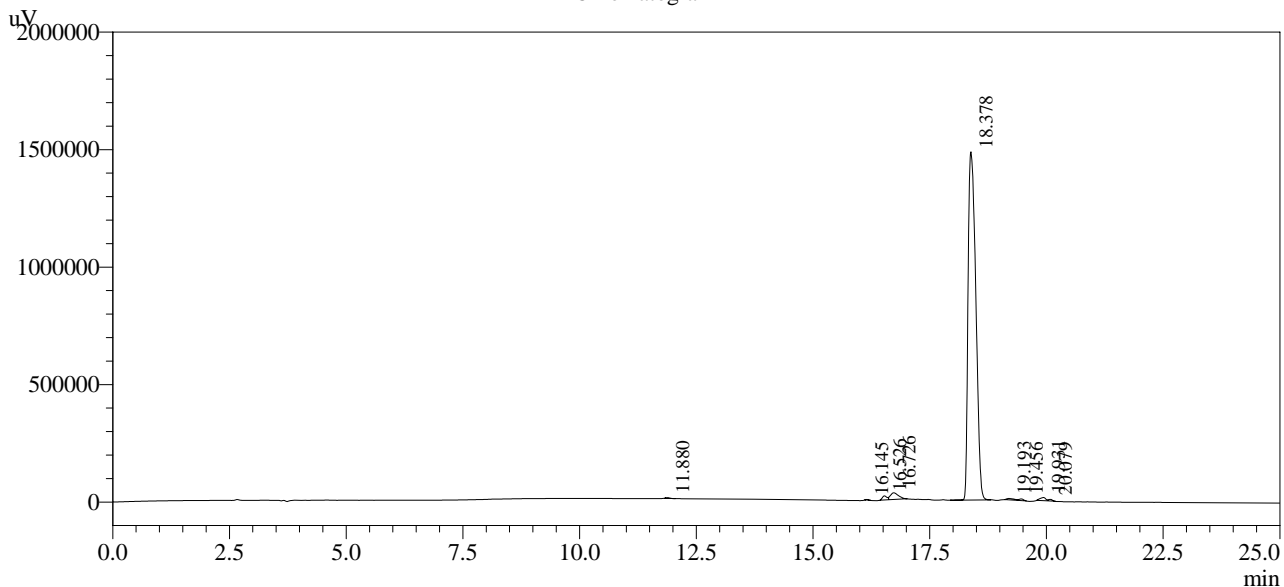

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.880	9631	1795	0.054
2	16.145	9217	2378	0.052
3	16.526	120371	17210	0.676
4	16.726	335369	28342	1.883
5	18.378	17076011	1482137	95.852
6	19.193	67196	5560	0.377
7	19.456	42912	6710	0.241
8	19.931	117352	13316	0.659
9	20.079	36954	6980	0.207
Total		17815014	1564428	100.000