

Sample Name : Octreotide (SMS 201-995)  
 Cat. No. : RP10222  
 Lot. No. : PE9841606

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

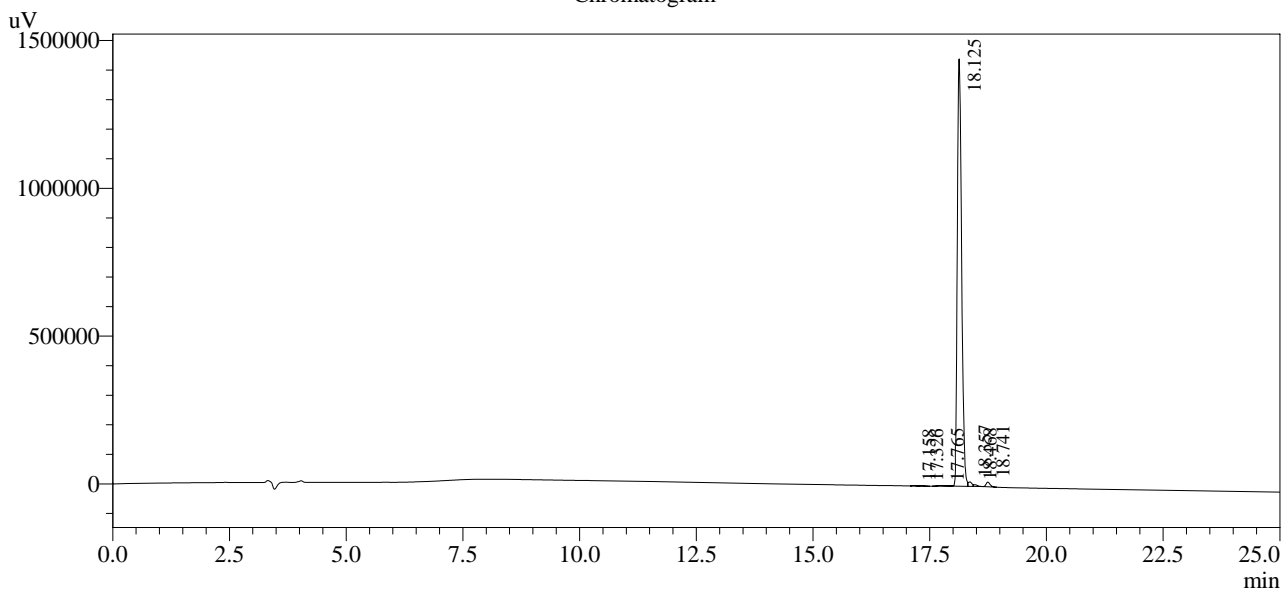

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.158	5325	1173	0.056
2	17.326	6483	998	0.068
3	17.765	19014	2199	0.199
4	18.125	9304963	1445611	97.533
5	18.357	79783	14916	0.836
6	18.468	31226	5573	0.327
7	18.741	93500	15765	0.980
Total		9540293	1486235	100.000