

Sample Name : Interleukin (IL)-6 Receptor  
 Cat No. : RP11738  
 Lot No. : PE9001606

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
40.00	Pumps	Pump B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

mV

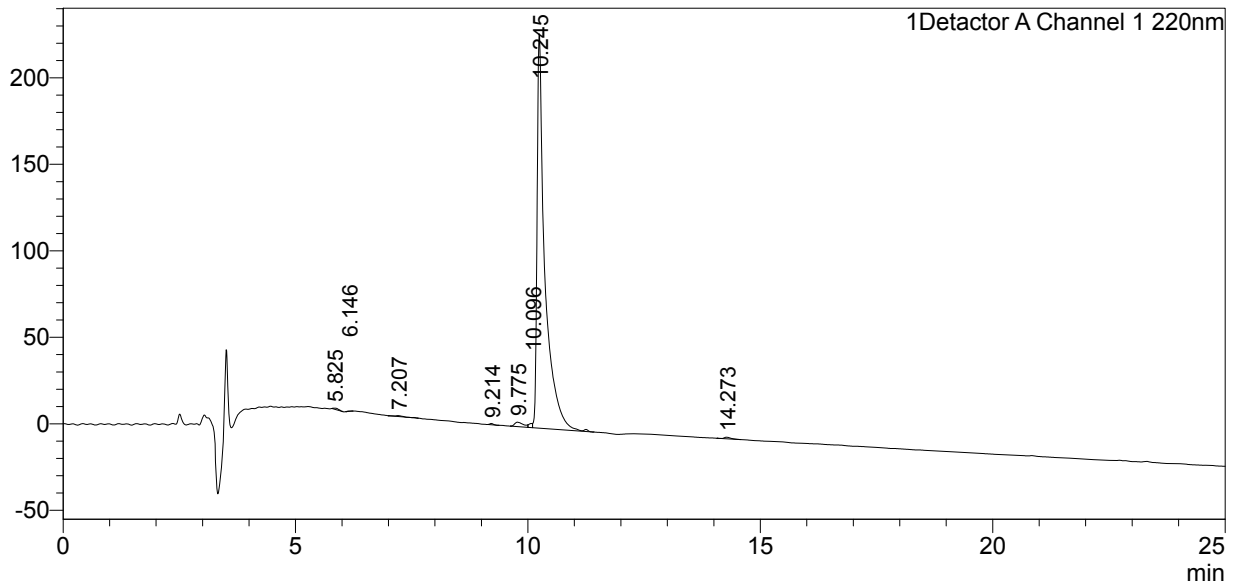

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.825	5903	501	0.216
2	6.146	1141	225	0.042
3	7.207	6692	566	0.244
4	9.214	3465	726	0.127
5	9.775	34607	2592	1.264
6	10.096	12857	2447	0.469
7	10.245	2665519	227954	97.333
8	14.273	8381	926	0.306
Total		2738566	235938	100.000