

Sample Name : AMARA peptide  
 Cat. No. : RP20472  
 Lot. No. : PE8401608


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

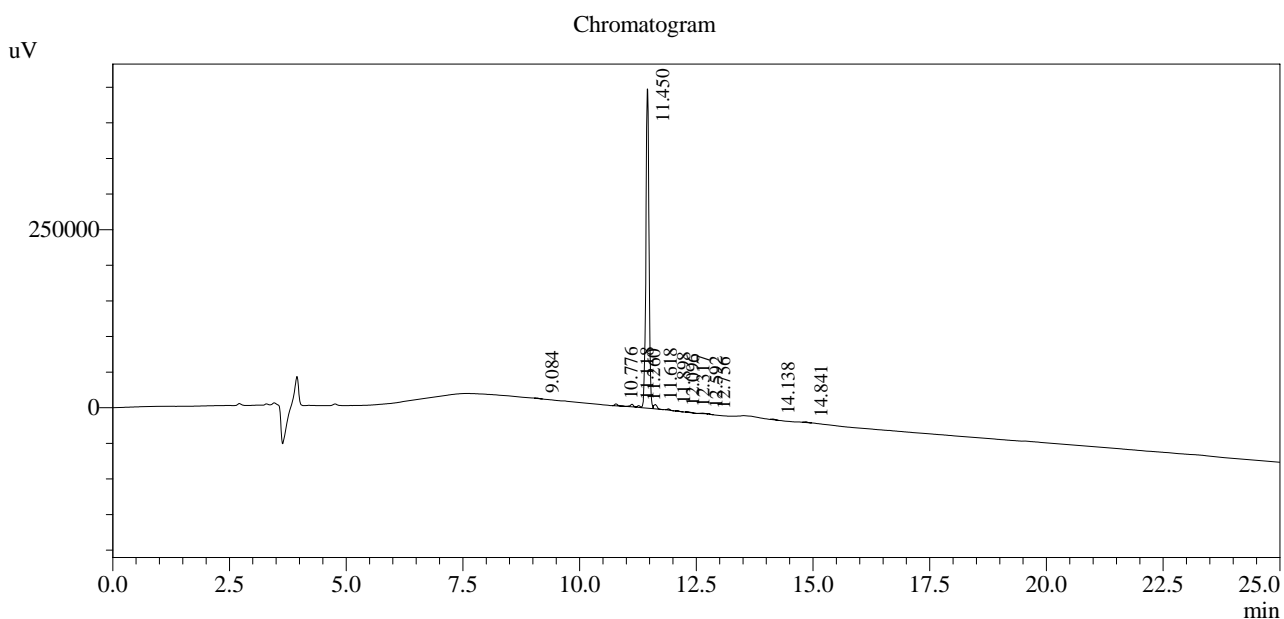

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.084	2602	636	0.120
2	10.776	14413	2739	0.664
3	11.118	17361	3660	0.800
4	11.260	10257	2426	0.473
5	11.450	2066327	448401	95.240
6	11.618	28979	6076	1.336
7	11.898	7245	1763	0.334
8	12.096	3545	864	0.163
9	12.317	4529	825	0.209
10	12.592	3796	587	0.175
11	12.756	1850	513	0.085
12	14.138	4046	971	0.186
13	14.841	4656	1053	0.215
Total		2169606	470514	100.000