

Sample Name :Exendin-4  
 Cat No.: RP10874  
 Lot No.: E4403919L  
 Time Processed :8:35:39  
 Month-Day-Year Processed :12/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

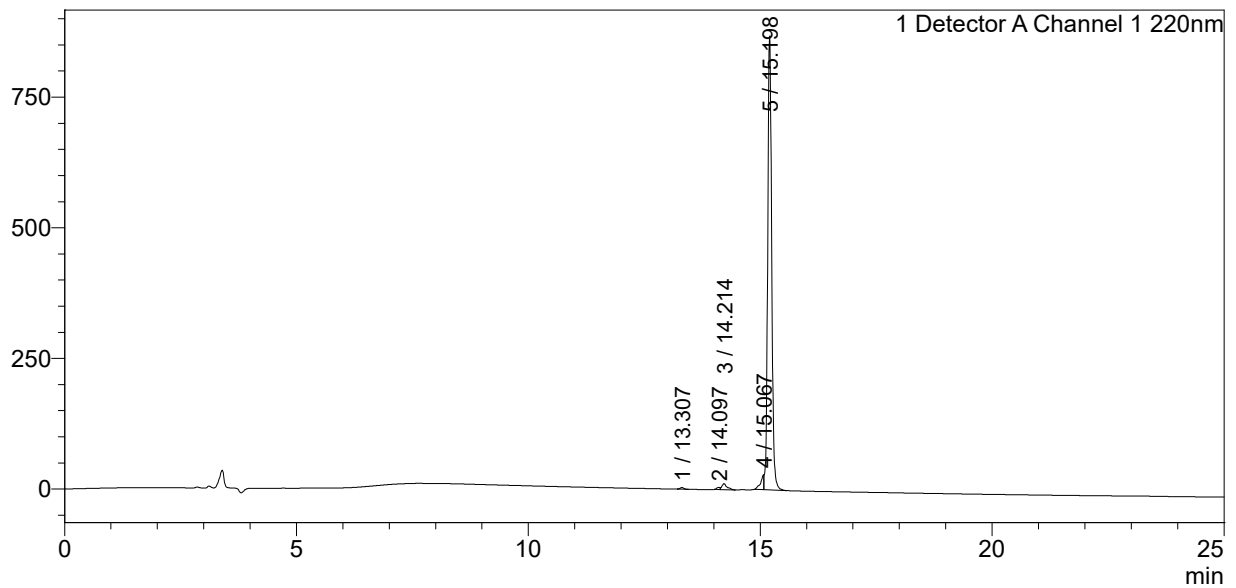

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.307	17575	3271	0.324
2	14.097	20841	4177	0.385
3	14.214	87474	11546	1.615
4	15.067	132938	27846	2.454
5	15.198	5159109	868800	95.223
Total		5417938	915640	100.000