

Sample Name : LCMV gp33-41
 Cat. No. : RP20257
 Lot. No. : PE1711607

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

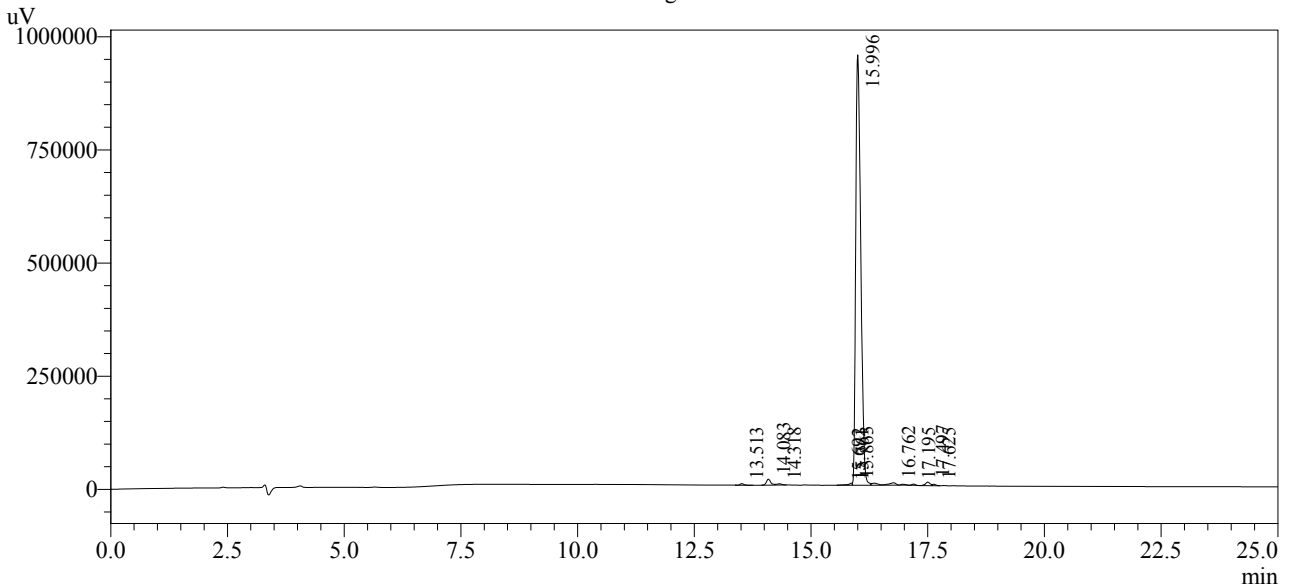

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.513	19161	3539	0.256
2	14.083	85675	13305	1.144
3	14.318	19762	2650	0.264
4	15.692	5273	827	0.070
5	15.761	7049	1417	0.094
6	15.863	19192	4571	0.256
7	15.996	7139851	951042	95.368
8	16.762	107020	5139	1.429
9	17.195	11817	2591	0.158
10	17.497	56366	7995	0.753
11	17.625	15465	3190	0.207
Total		7486629	996266	100.000