

Sample Name : N-Boc-Phe-Leu-Phe-Leu-Phe
 Sample ID : C7258BF200-1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
35.00	Pumps	Pump B Conc.	95
41.00	Pumps	Pump B Conc.	95
41.01	Pumps	Pump B Conc.	5
50.00	Pumps	Pump B Conc.	5
50.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

mV

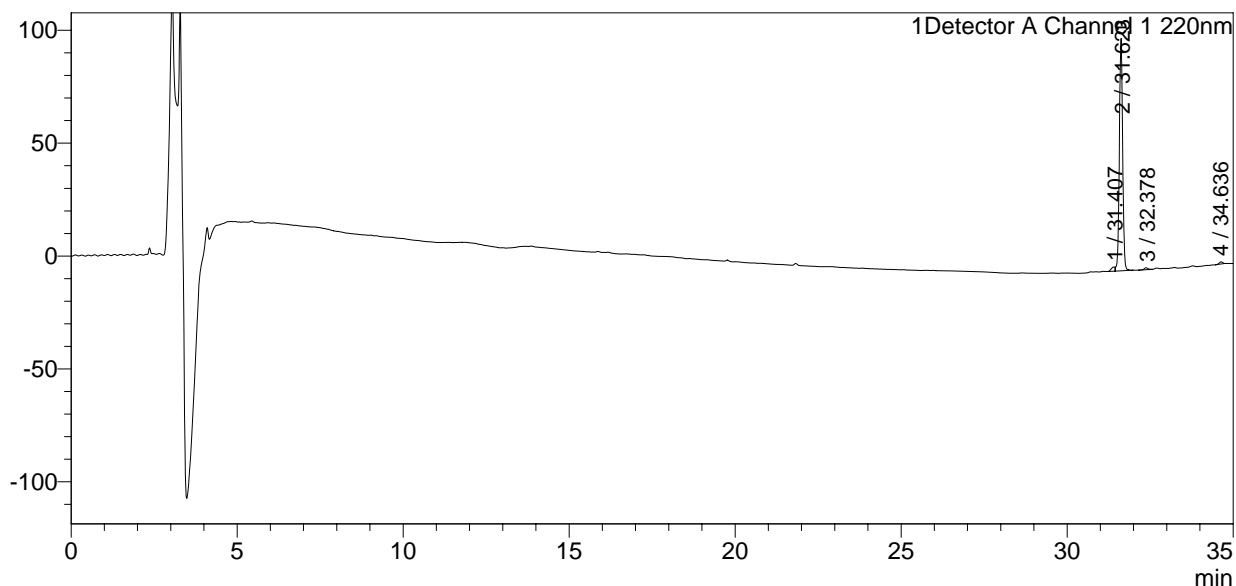

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	31.407	14667	1845	1.983
2	31.623	710898	102931	96.117
3	32.378	6549	847	0.886
4	34.636	6847	923	0.926
5	49.962	659	114	0.089
Total		739621	106660	100.000