


Mass Spectrum

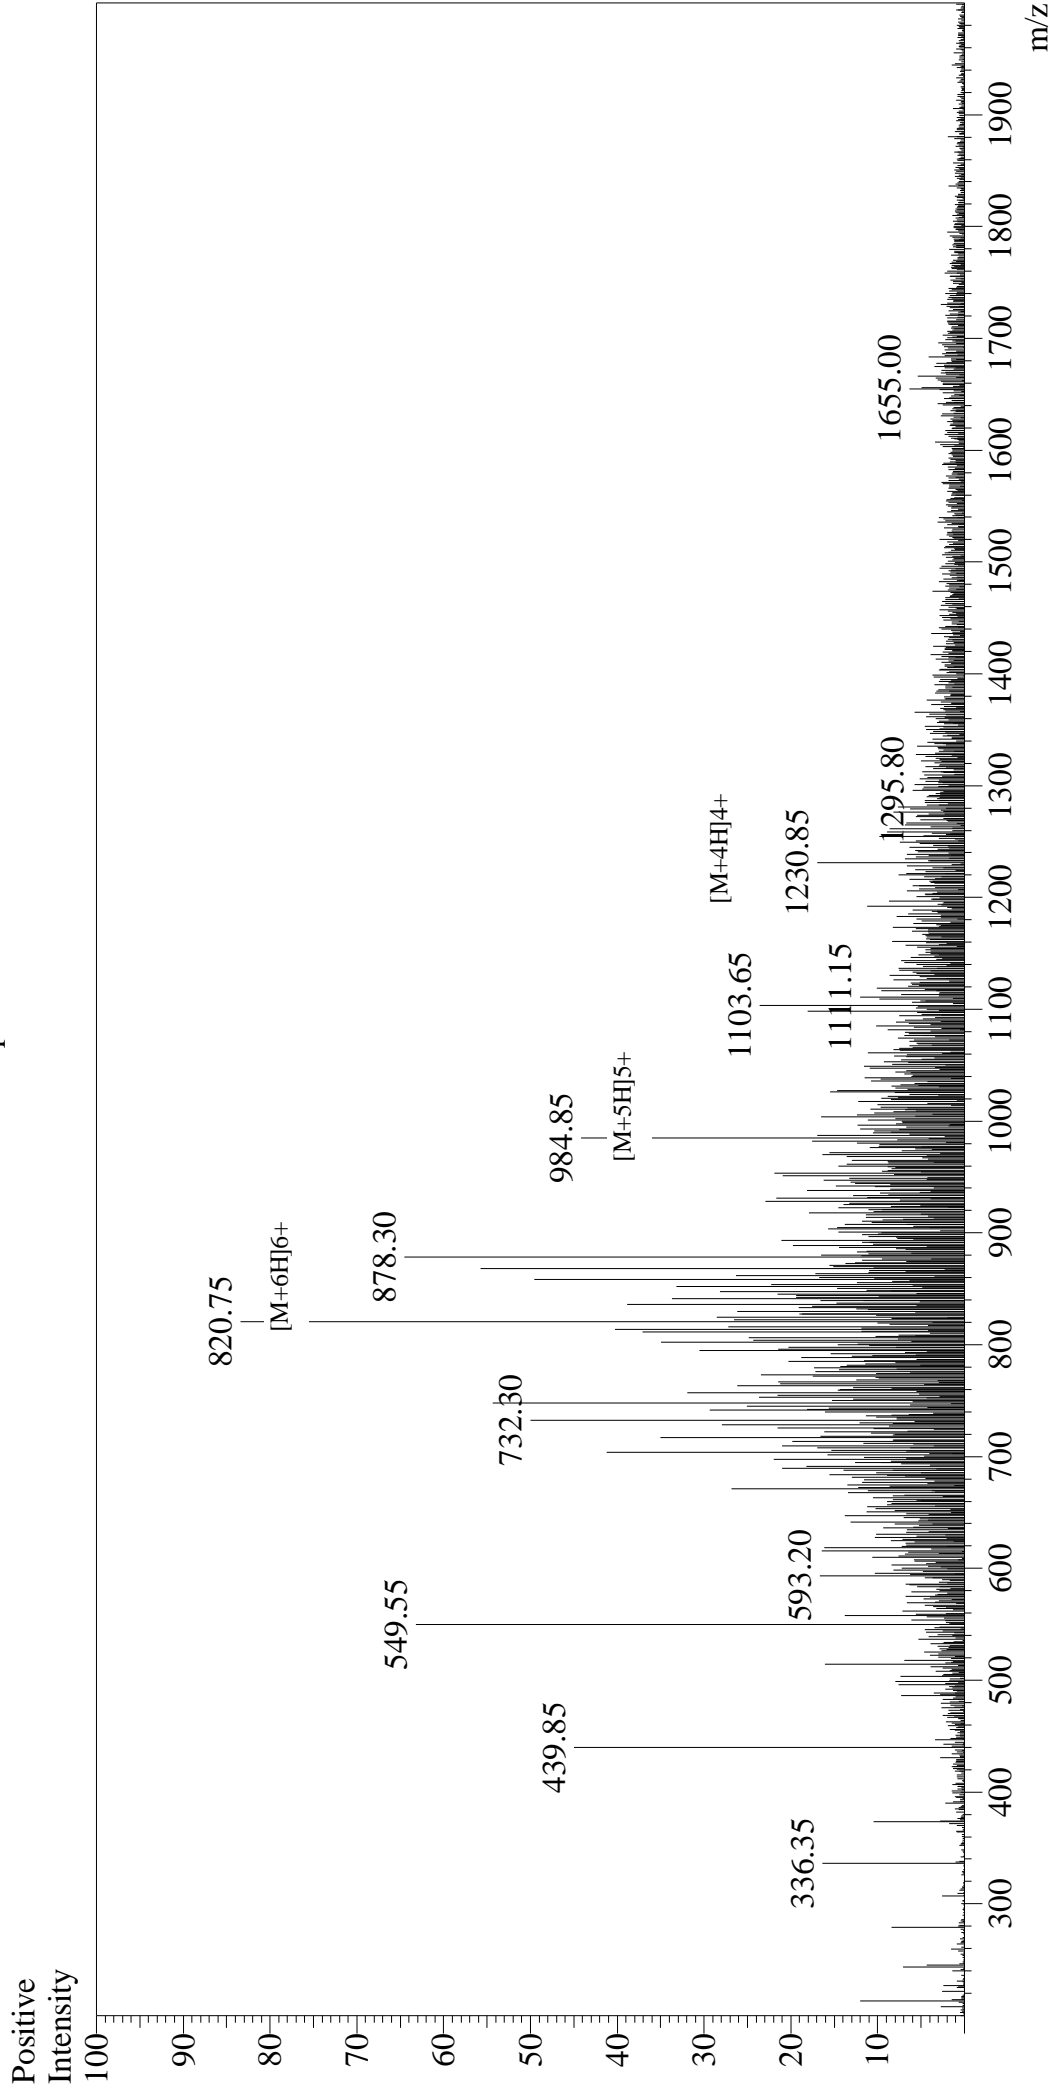

Sample Information

User : Gary
Month-Day Processed : 03/16/16
Time Processed : 14:49:20
Injection Volume : 0.2
Sample Name : BNP(1-45), mouse
Cat No. : RP20365
Lot No. : PE2661601
Theoretical MW : 4919.60
Observed MW : 4918.50

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH