


Mass Spectrum

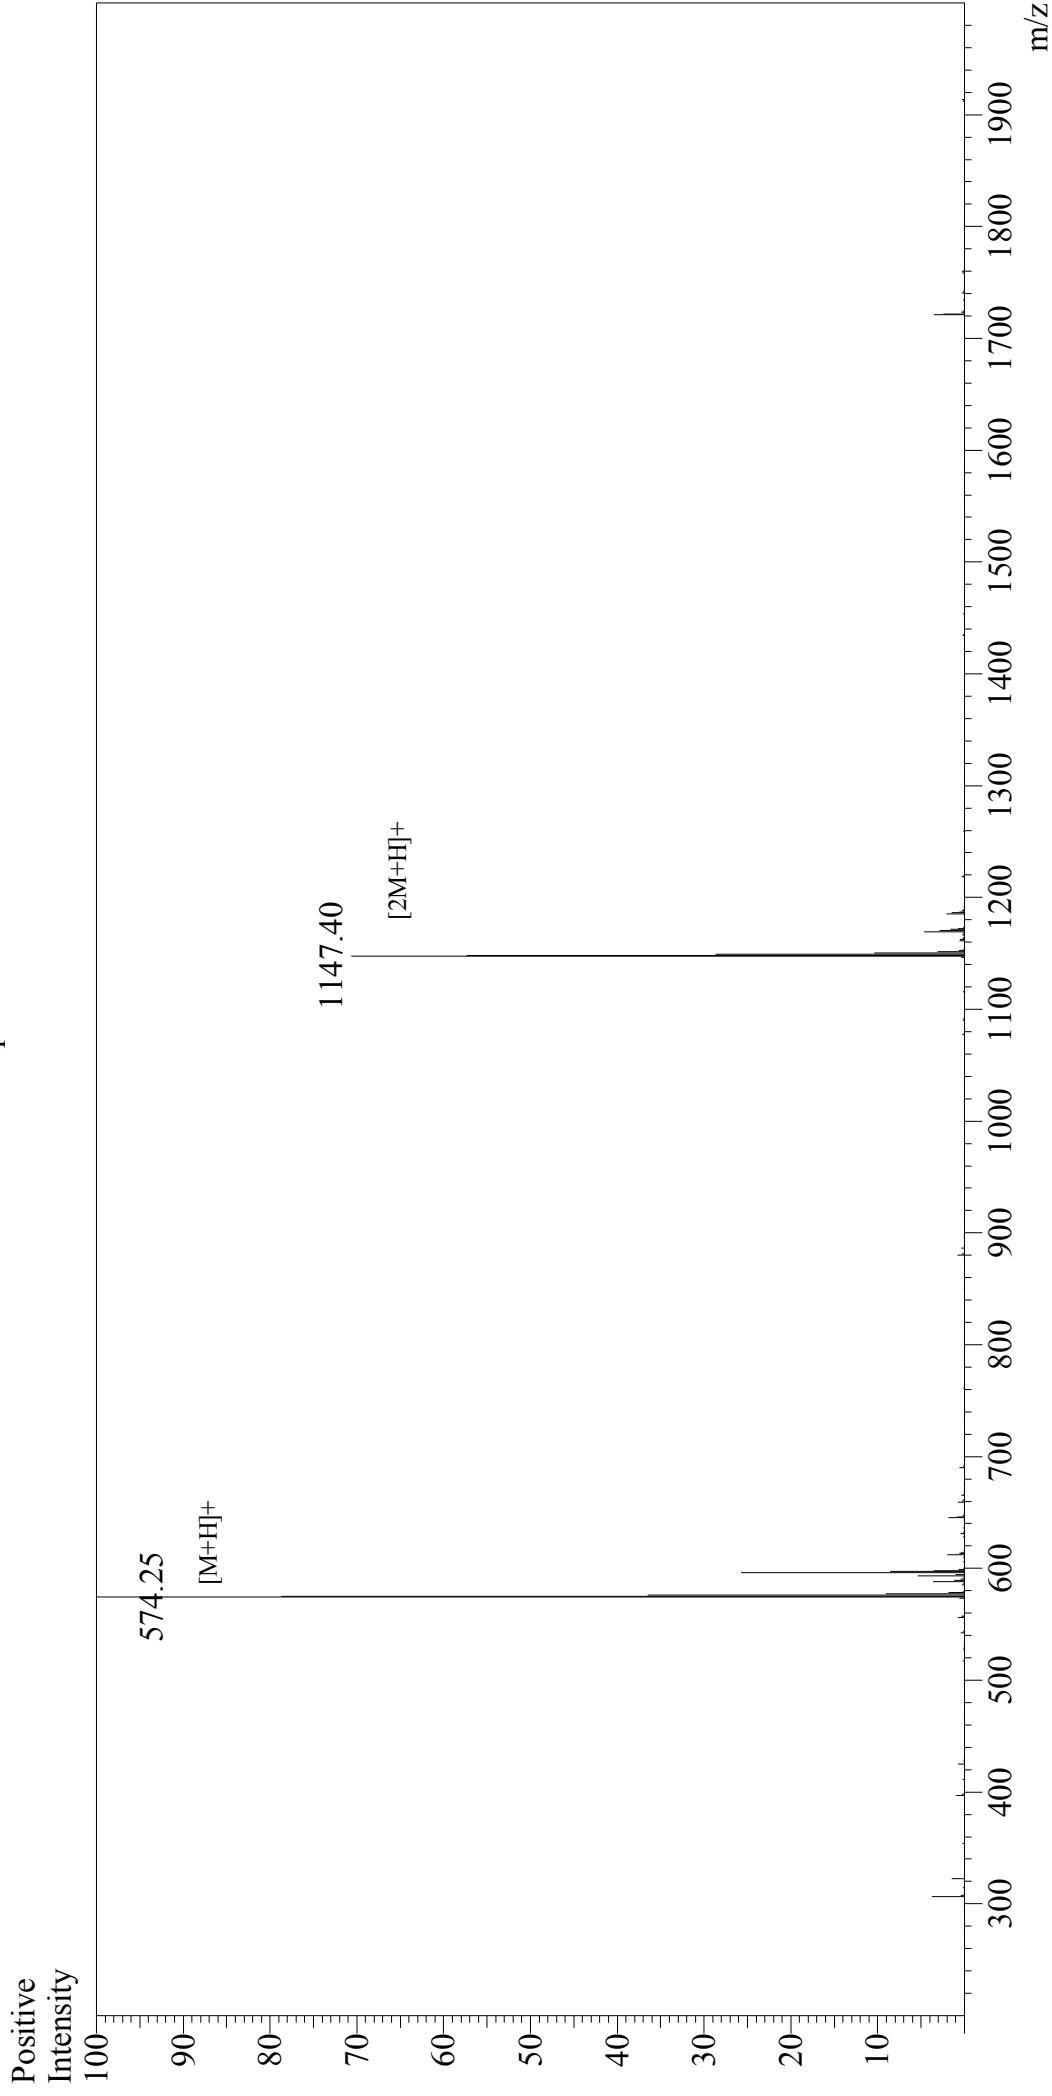

Sample Information

User : Gary
Month-Day Processed : 08/15/16
Time Processed : 8:11:49
Injection Volume : 0.2
Sample Name : [Met⁵-Enkephalin
Cat No. : RPI0886
Lot No. : PE4561608
Theoretical MW : 573.66
Observed MW : 573.25

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH