

Sample Name : Competence-Stimulating Peptide-12261
 Cat. No. : RP20427
 Lot. No. : PE9891608

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

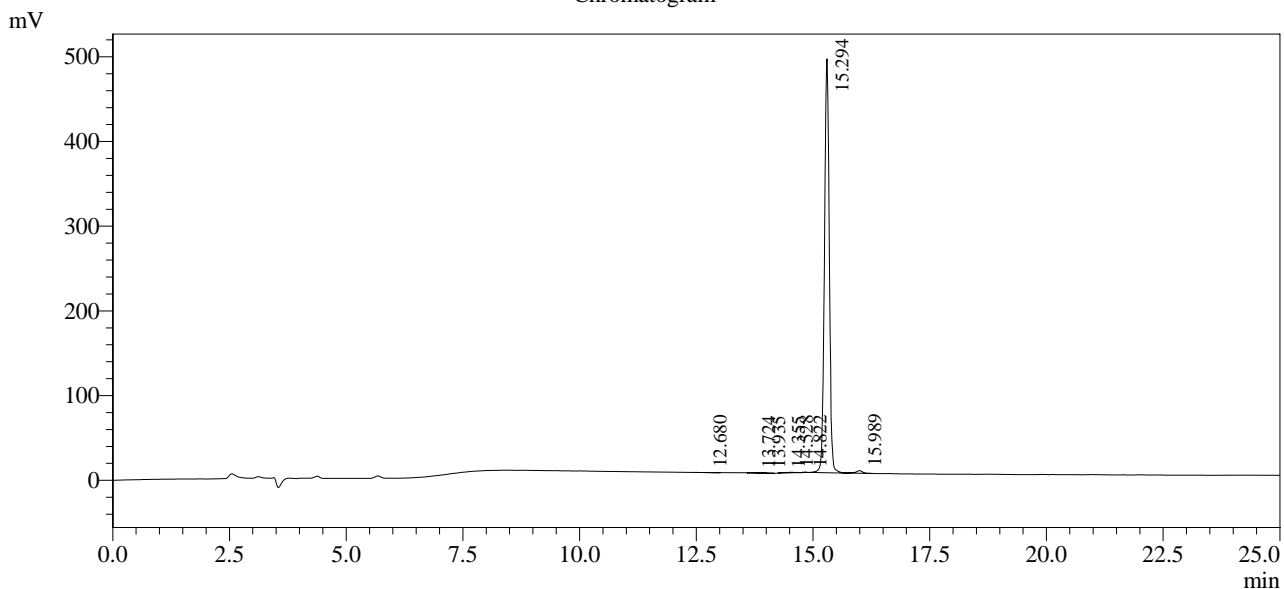

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.680	2467	382	0.069
2	13.724	2026	342	0.057
3	13.935	1687	337	0.047
4	14.355	3250	470	0.091
5	14.528	5608	567	0.157
6	14.822	3159	599	0.088
7	15.294	3527620	488659	98.594
8	15.989	32126	3092	0.898
Total		3577942	494446	100.000