

Sample Name : IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E0047423H
 Time Processed :12:01:26
 Month-Day-Year Processed :08/27/2023
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
 Equipment: GR11010440

<Chromatogram>

mV

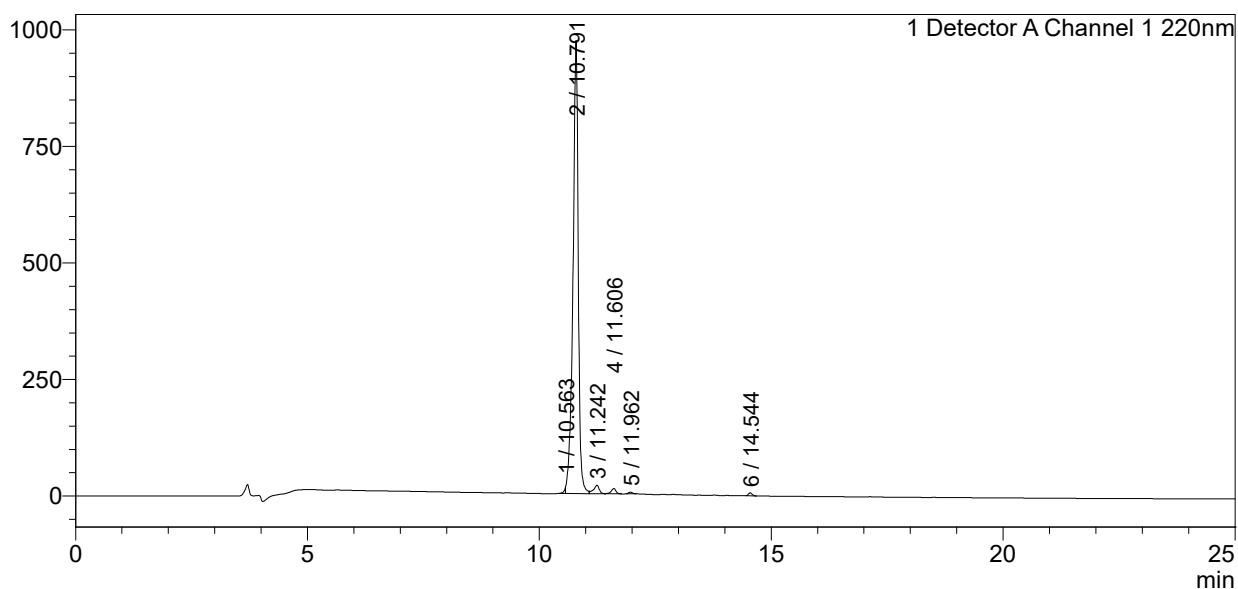

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.563	31076	11464	0.387
2	10.791	7714210	972300	96.017
3	11.242	156318	18085	1.946
4	11.606	80486	11473	1.002
5	11.962	18640	3327	0.232
6	14.544	33502	6263	0.417
Total		8034233	1022912	100.000