


Mass Spectrum

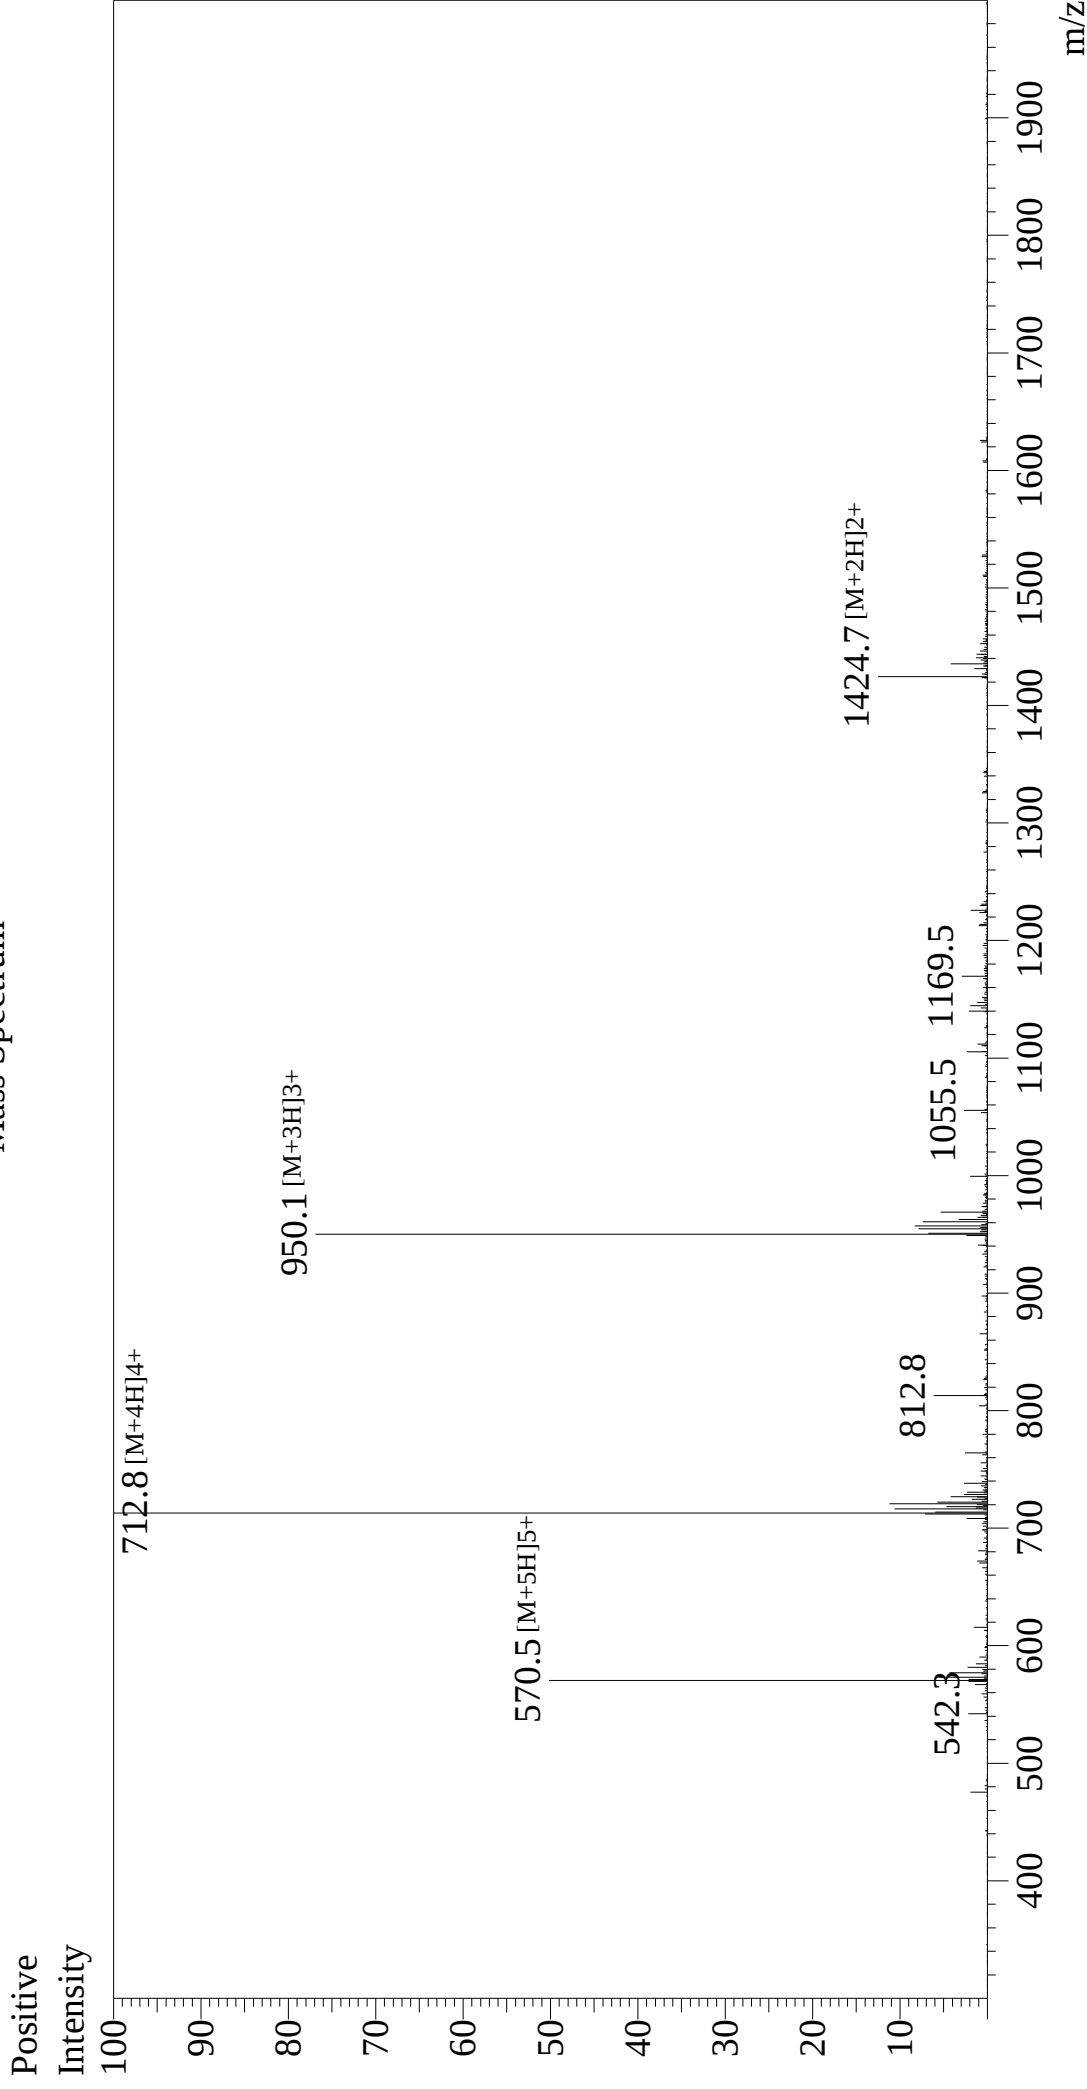

Sample Information

Month-Day Processed : 10/10/24
 Time Processed : 9:59:15 AM
 Injection Volume : 0.3
 Sample Name : Melittin,honey bee
 Cat No. : RP20415
 Lot No. : E0124624J
 Theoretical MW: 2847.50
 Observed MW : 2847.2

Interface :ESI
 Nebulizing Gas Flow :1.5L/min
 CDL Temp :250
 Block Temp :200

Equipment :ZJ22010150
 Interface Bias : +4.5 kV
 Drying Gas Flow :5 L/min
 T.Flow :0.2 ml/min
 B.conc :50%H₂O/50%M