


Mass Spectrum

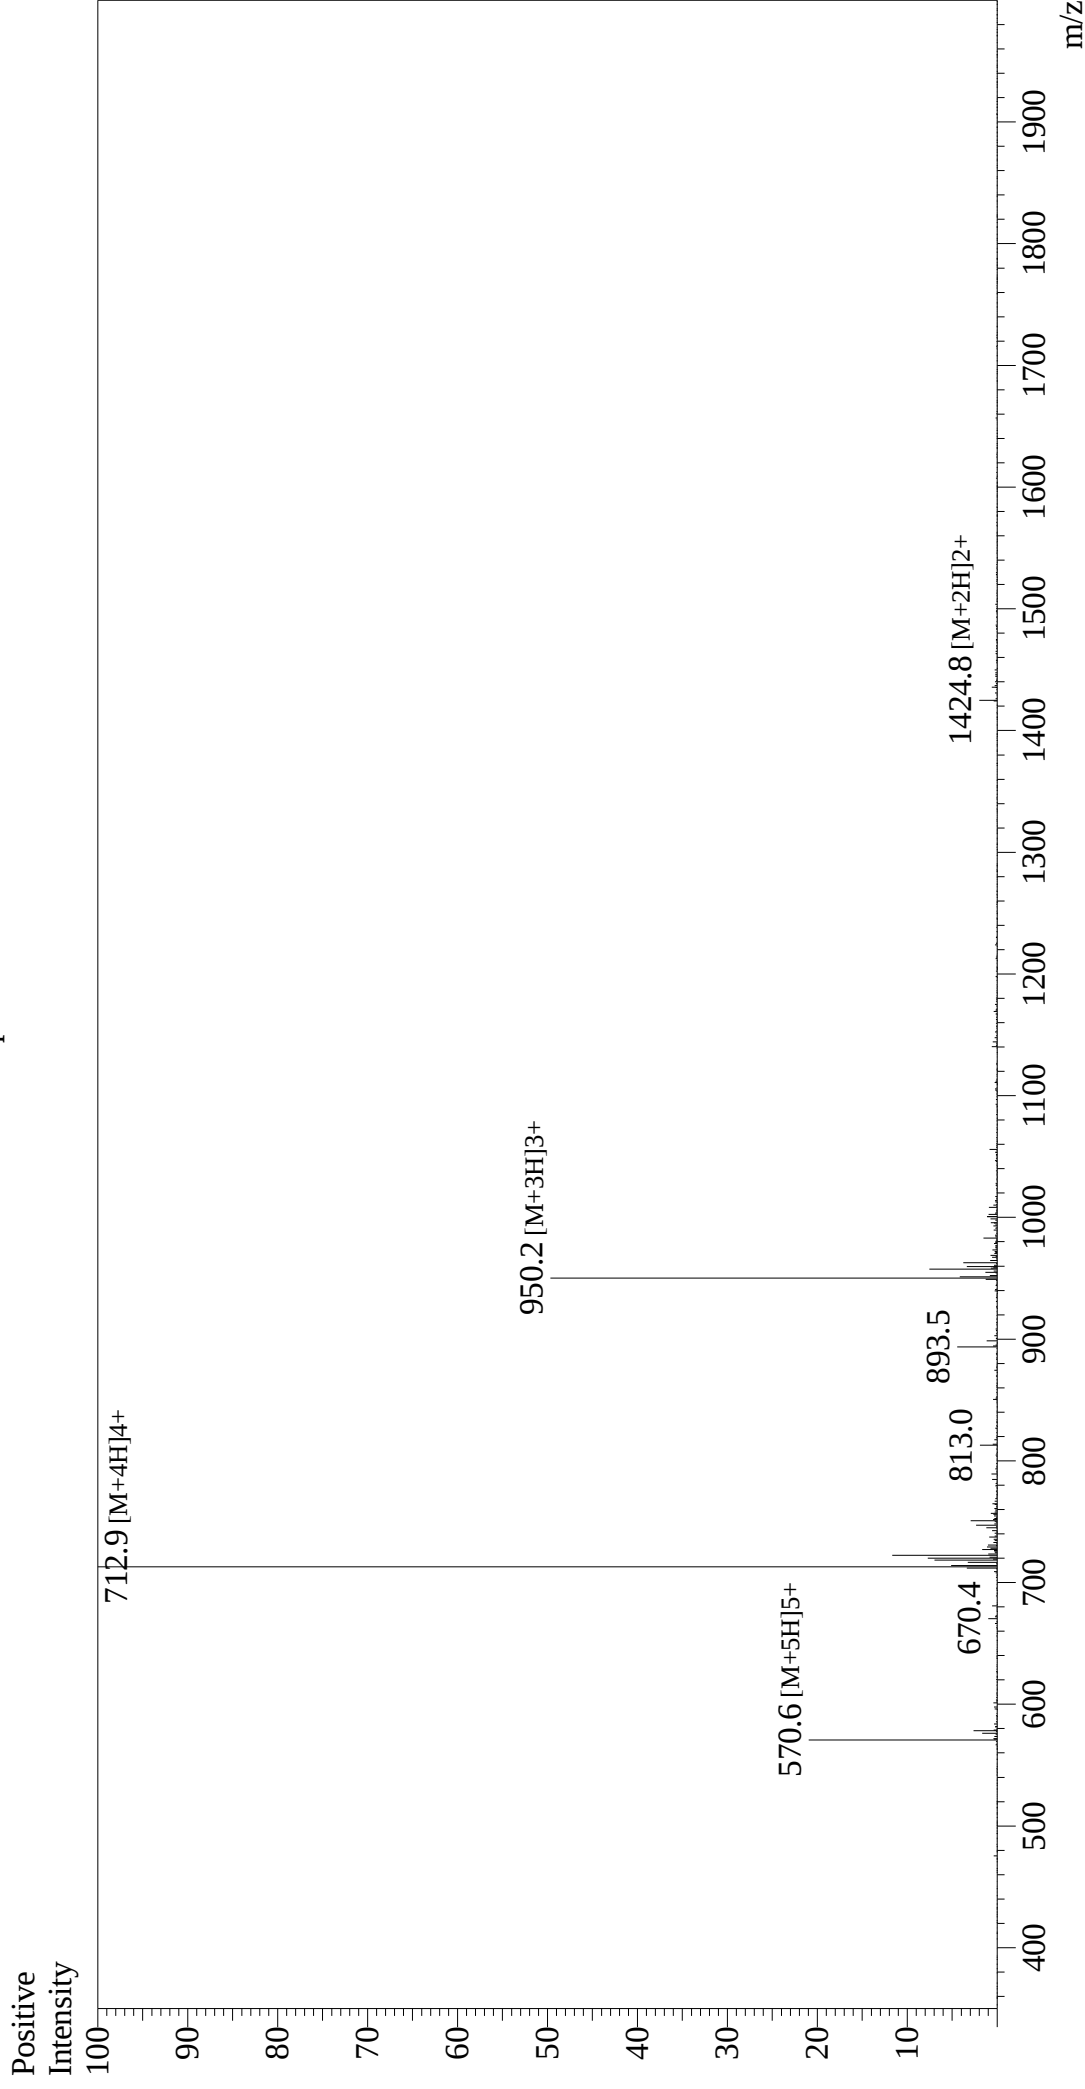

Sample Information

Month-Day Processed :	11/01/22	Equipment	: ZJ21010035
Time Processed :	20:51:34	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	: 5 L/min
Sample Name :	Melittin, honey bee	T.Flow	: 0.2 ml/min
Cat No. :	RP20415	B.conc	: 50% H ₂ O/50% MeOH
Lot No. :	E0155422J		
Theoretical MW : 2847.50			
Observed MW : 2847.6			