


Mass Spectrum

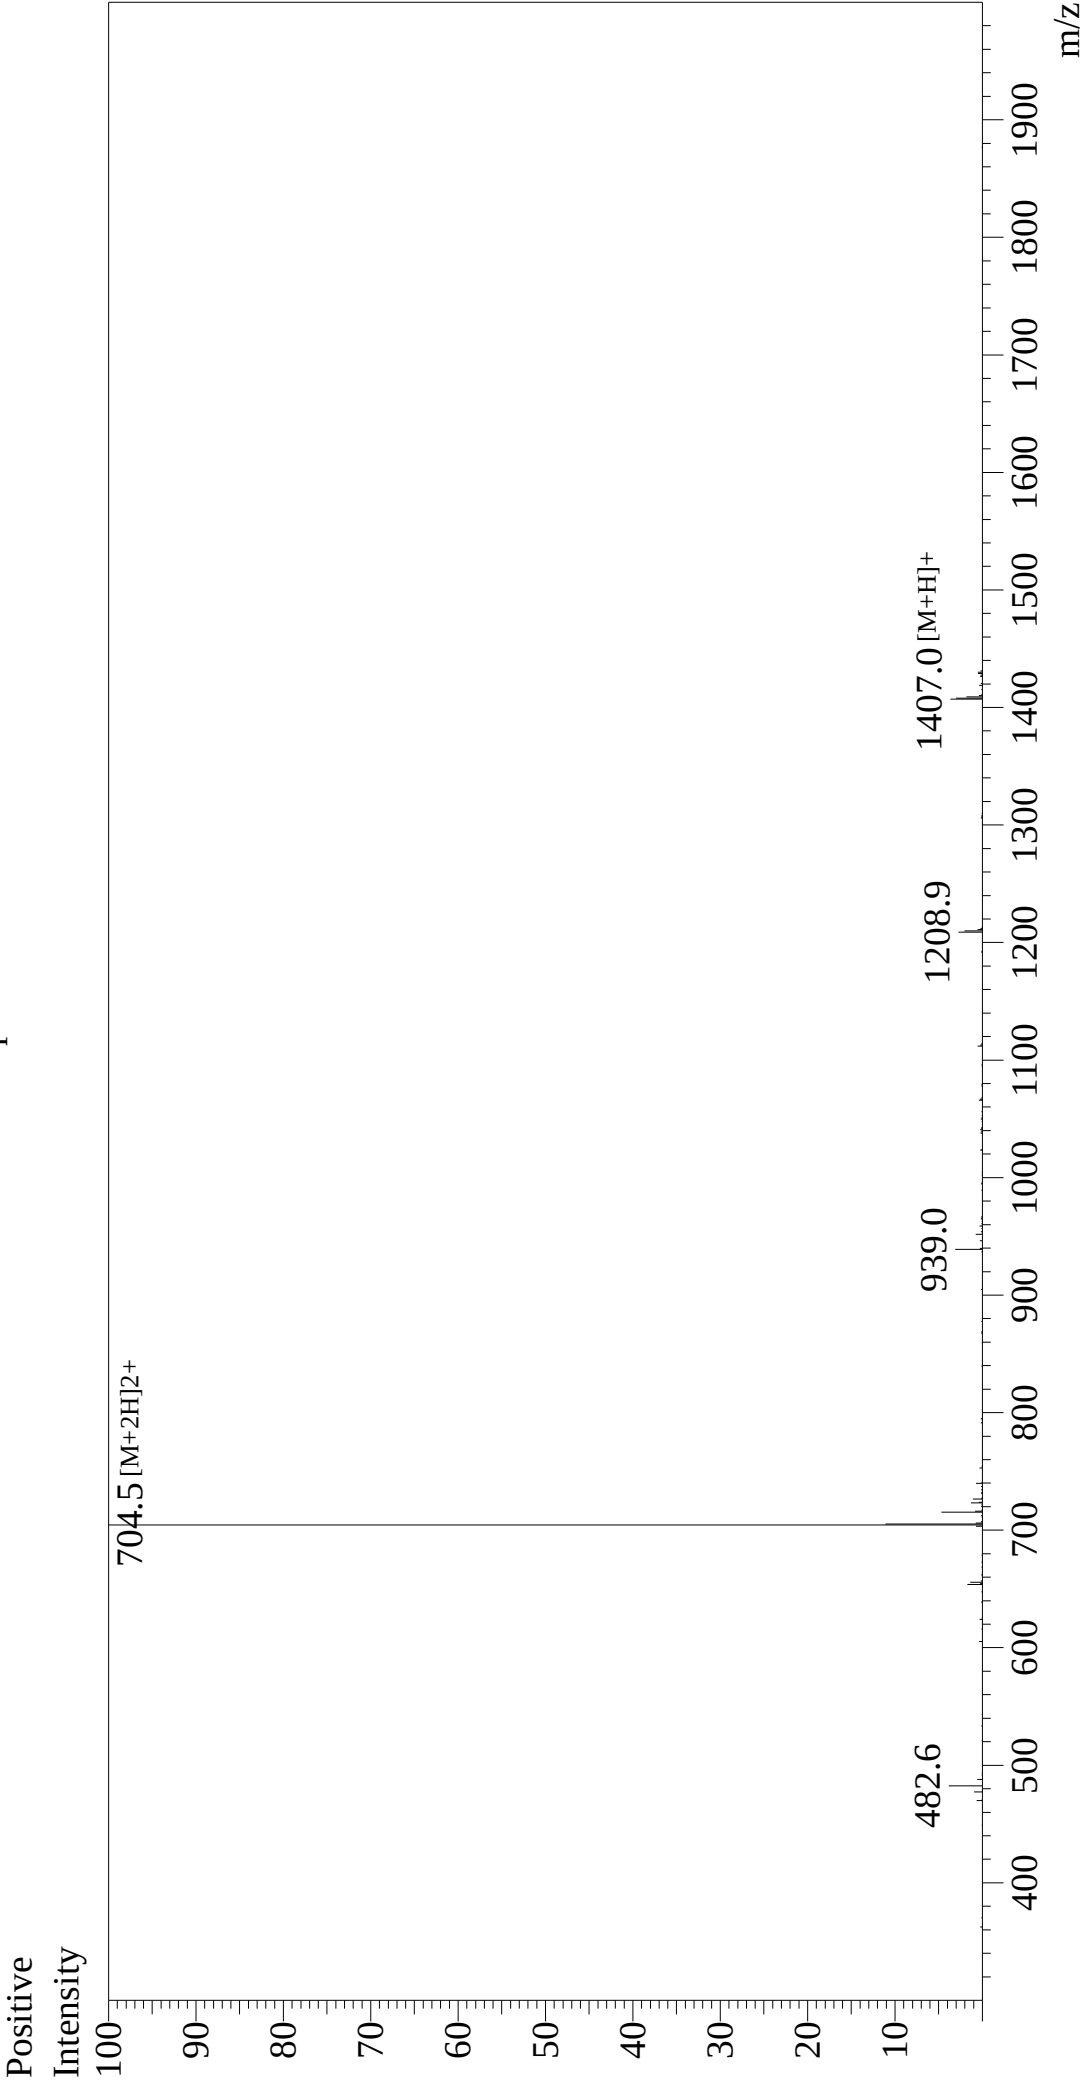

Sample Information		Equipment	
Month-Day Processed :	08/15/22	Interface	:ZJ22010150
Time Processed :	2:35:44 PM	Nebulizing Gas Flow	: +4.5 kV
Injection Volume :	0.1	CDL Temp	:5 L/min
Sample Name :	Hepatitis B Virus Core (128-140)	Block Temp	:0.2 ml/min
Cat No. :	RP17313		:50%H2O/50%M
Lot No. :	E0203422H		
Theoretical MW:1406.63			
Observed MW : 1407.0			