


Mass Spectrum

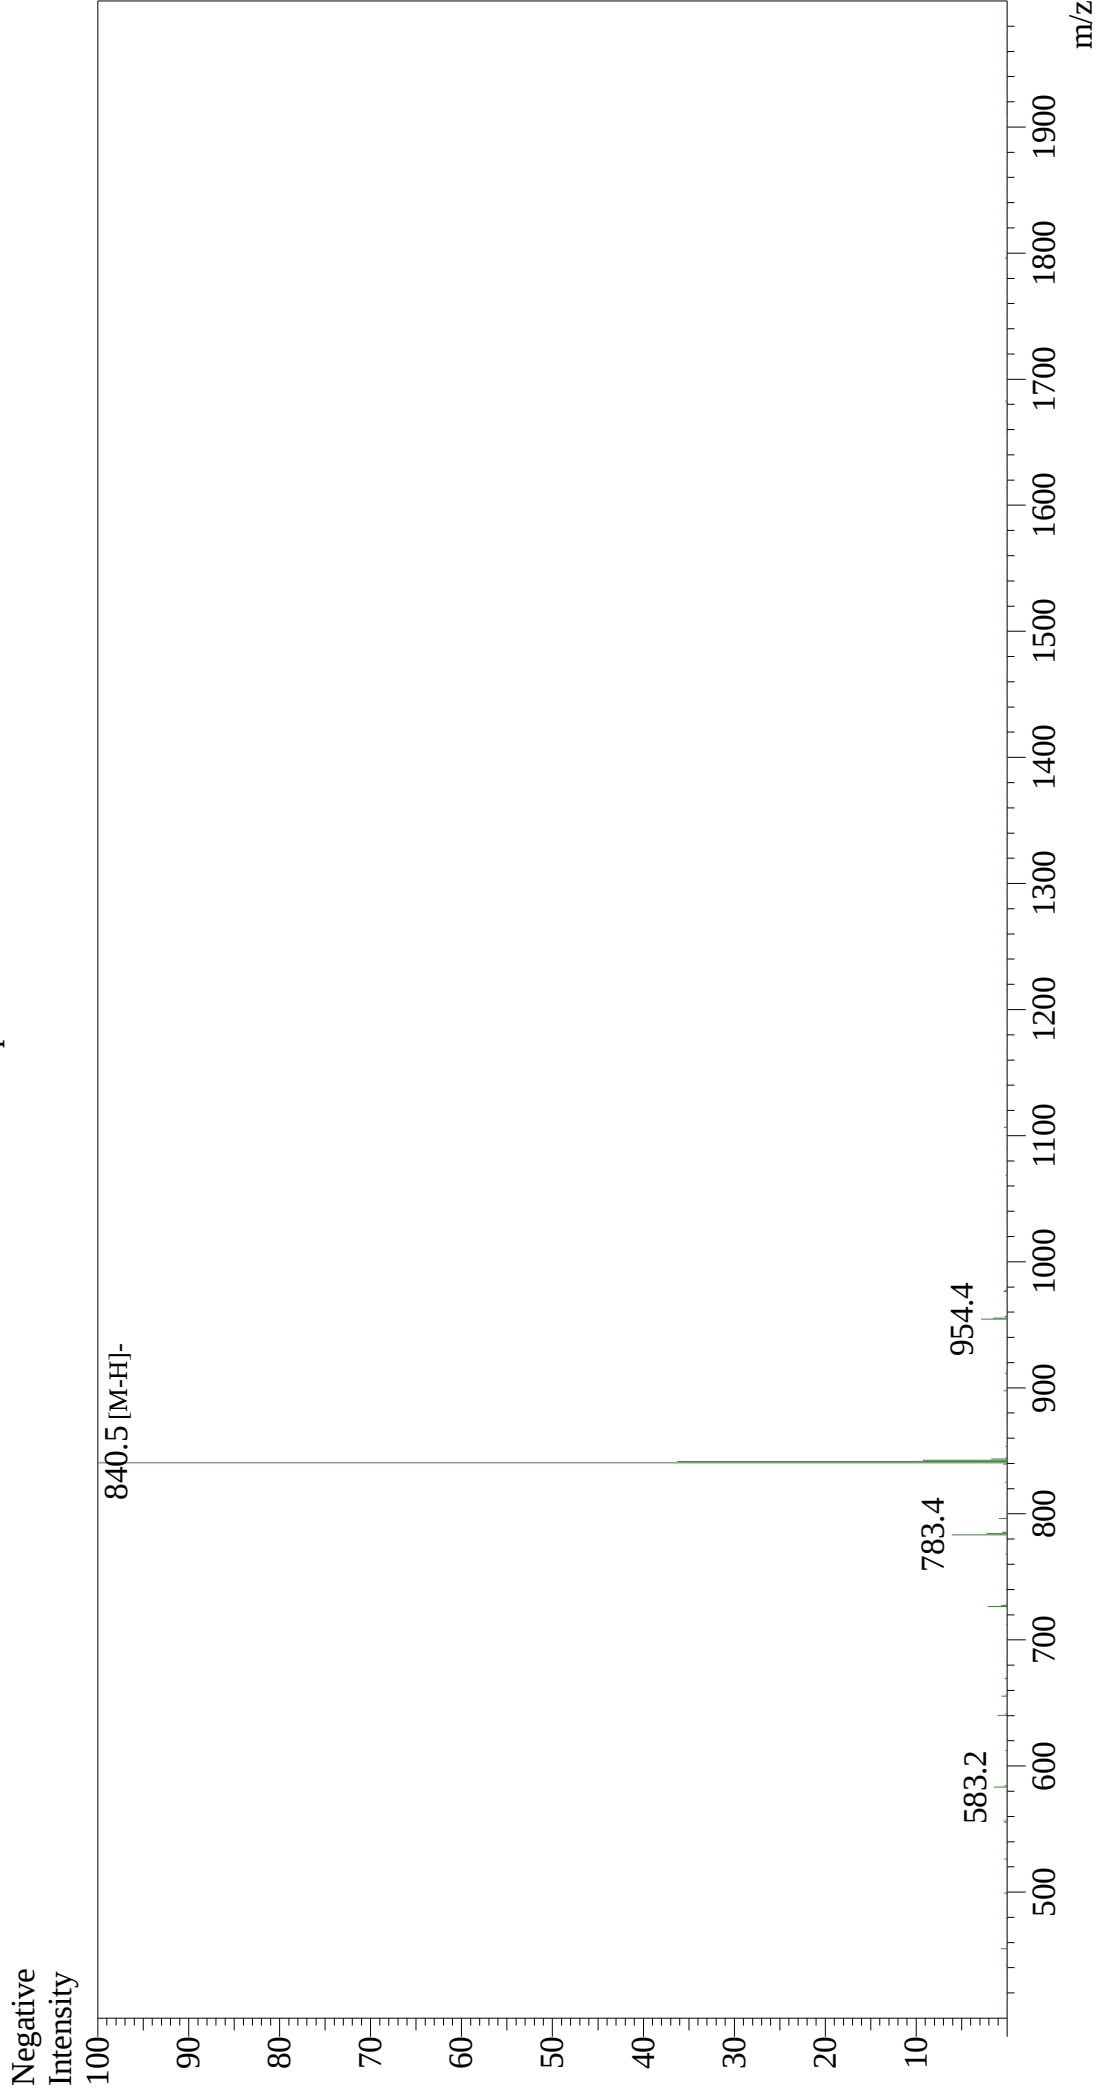

Sample Information

Month-Day Processed : 12/12/23

Time Processed : 18:44:57

Injection Volume : 0.3

Sample Name : KRAS WT Peptide (VVVGAGGVGK)

Cat No. : RP30235

Lot No. : E0219123L

Theoretical MW : 842.00

Observed MW : 841.5

Interface : ESI

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias : -3.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50%H₂O/50%MeOH

Equipment : ZJ21010035