


Mass Spectrum

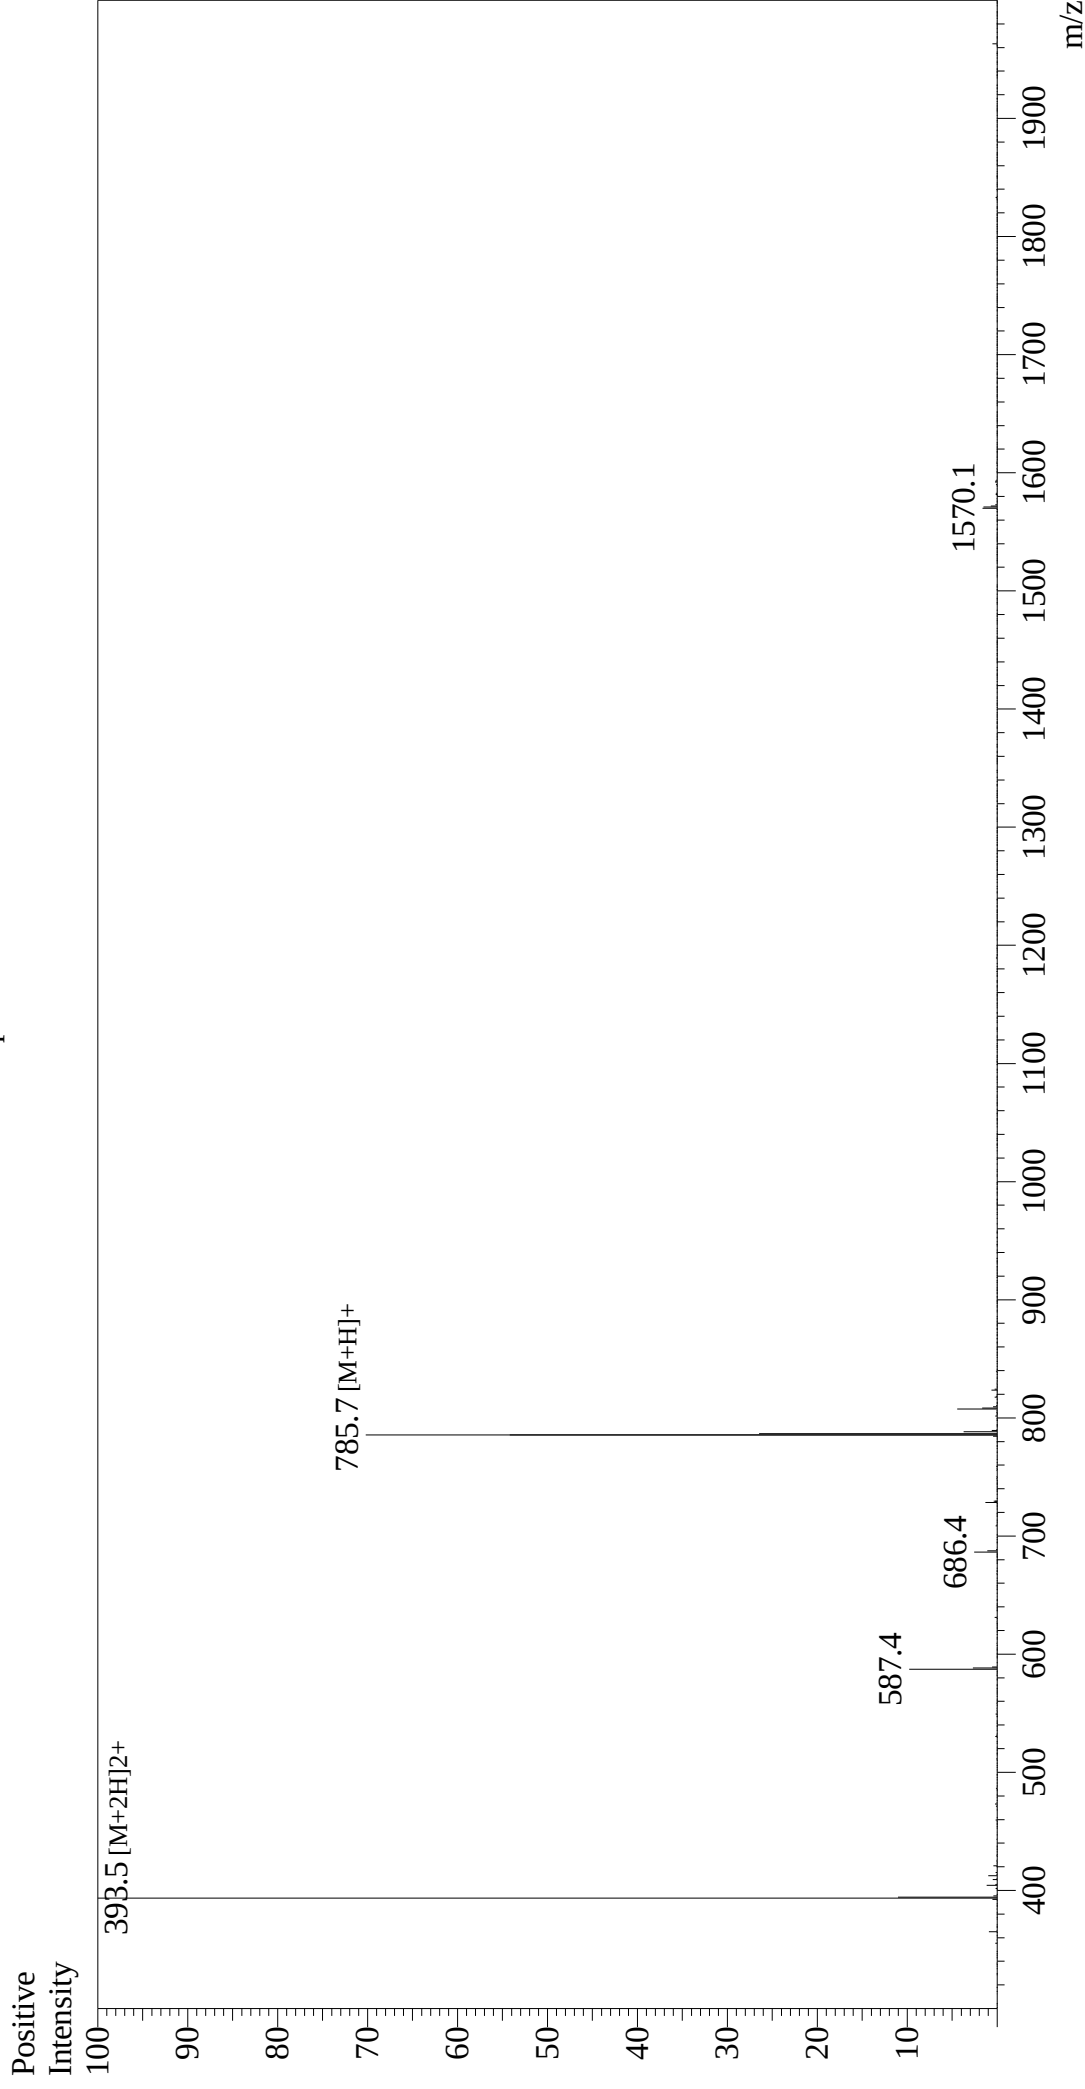

Sample Information

Month-Day Processed : 08/15/25
Time Processed : 10:16:36
Injection Volume : 0.3
Sample Name : KRAS G12V Peptide (VVGAVGVGK)
Cat No. : RP30228
Lot No. : E0447725H
Theoretical MW : 784.95
Observed MW : 785.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH