


# Mass Spectrum

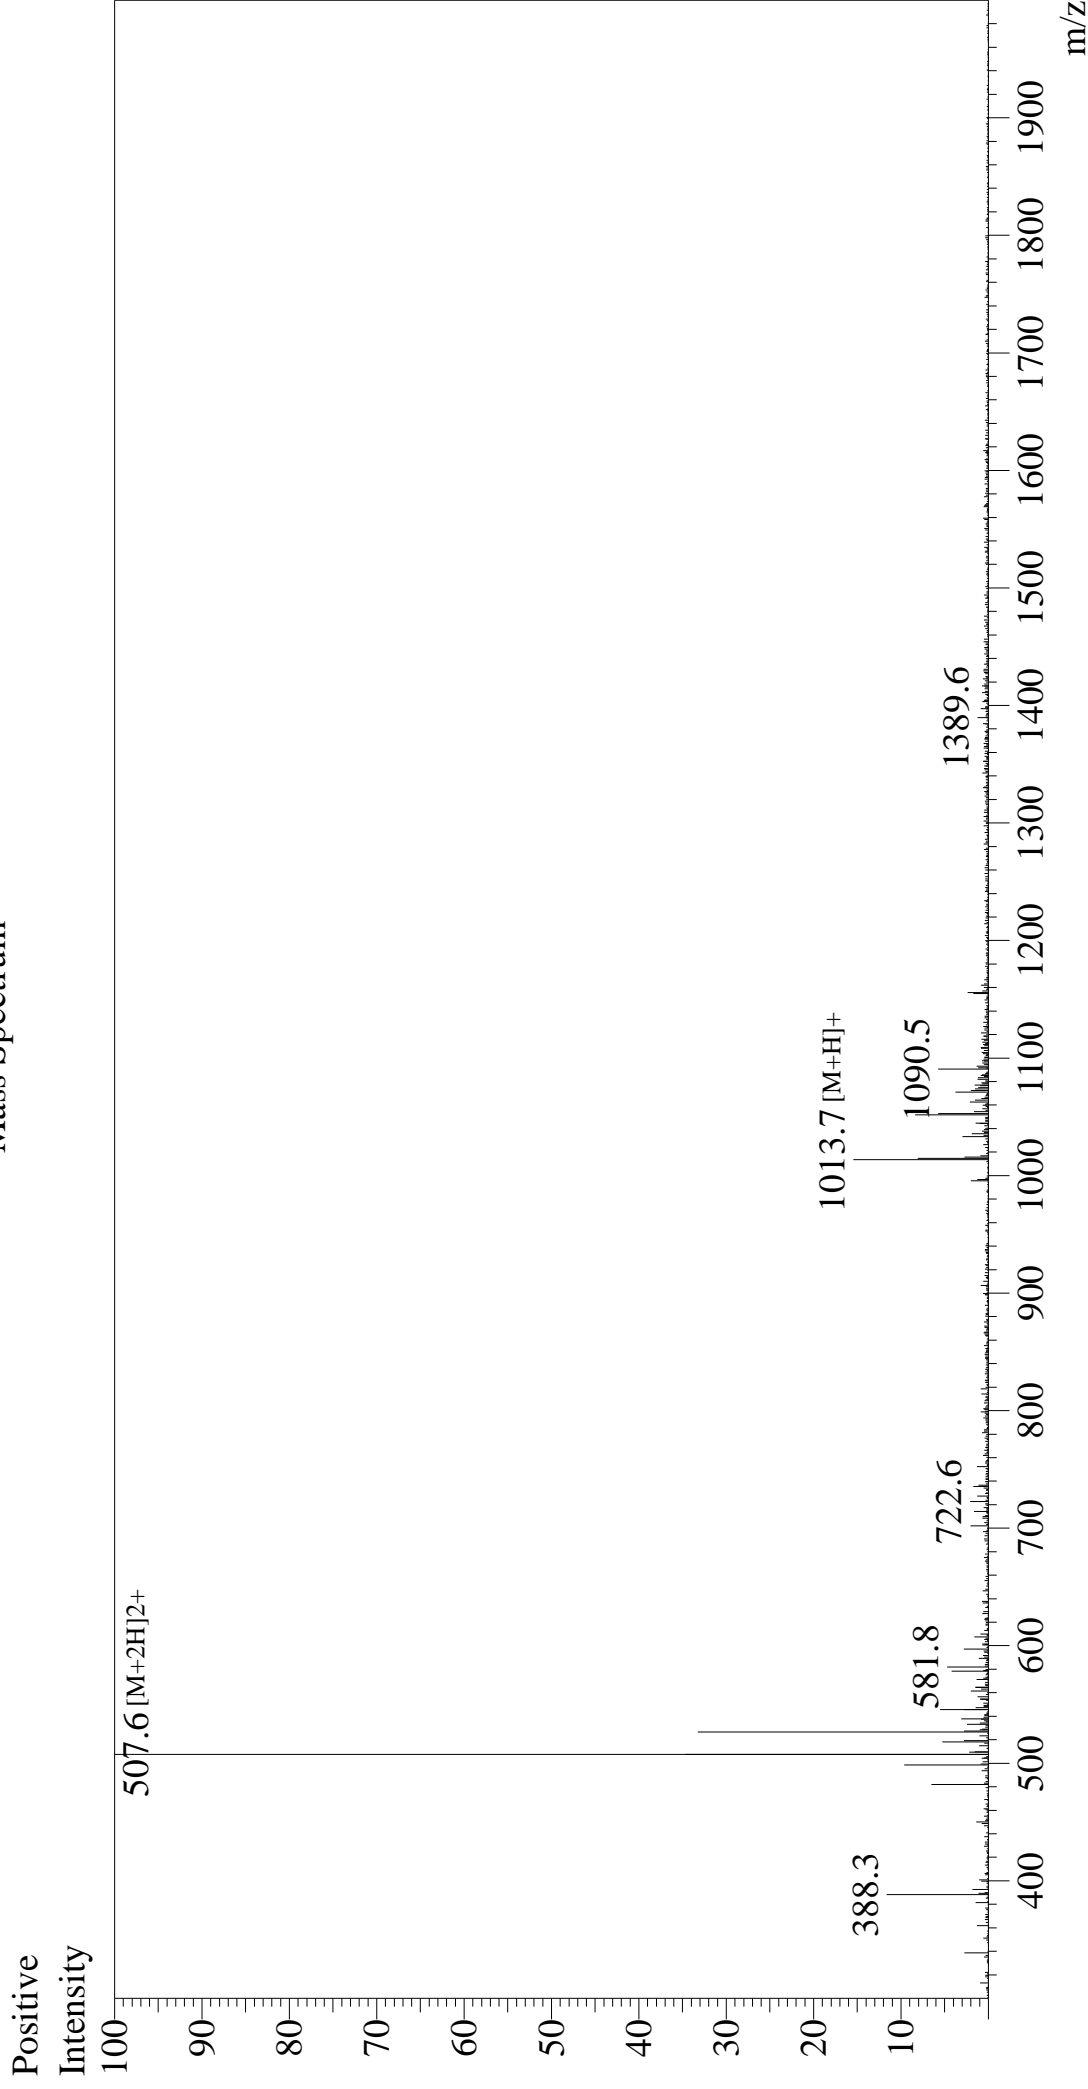

Sample Information		Equipment	
Month-Day Processed :	07/08/23	Interface	:ESI
Time Processed :	4:41:16 PM	Nebulizing Gas Flow	:1.5L/min
Injection Volume :	0.1	CDL Temp	:250
Sample Name :	DYKDDDDK Peptide	Block Temp	:200
Cat No. :	RP10586	Equipment	
Lot No. :	E0517723G	Interface Bias	: +4.5 kV
Theoretical MW : 1012.97		Drying Gas Flow	:5 L/min
Observed MW : 1013.2		T.Flow	:0.2 ml/min
		B.conc	:50% H2O/50% MeOH