

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat

Cat No. : RP11095

Lot No. : E0555125C

Time Processed :10:01:40

Month-Day-Year Processed :03/09/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ17010509

### <Chromatogram>

mV

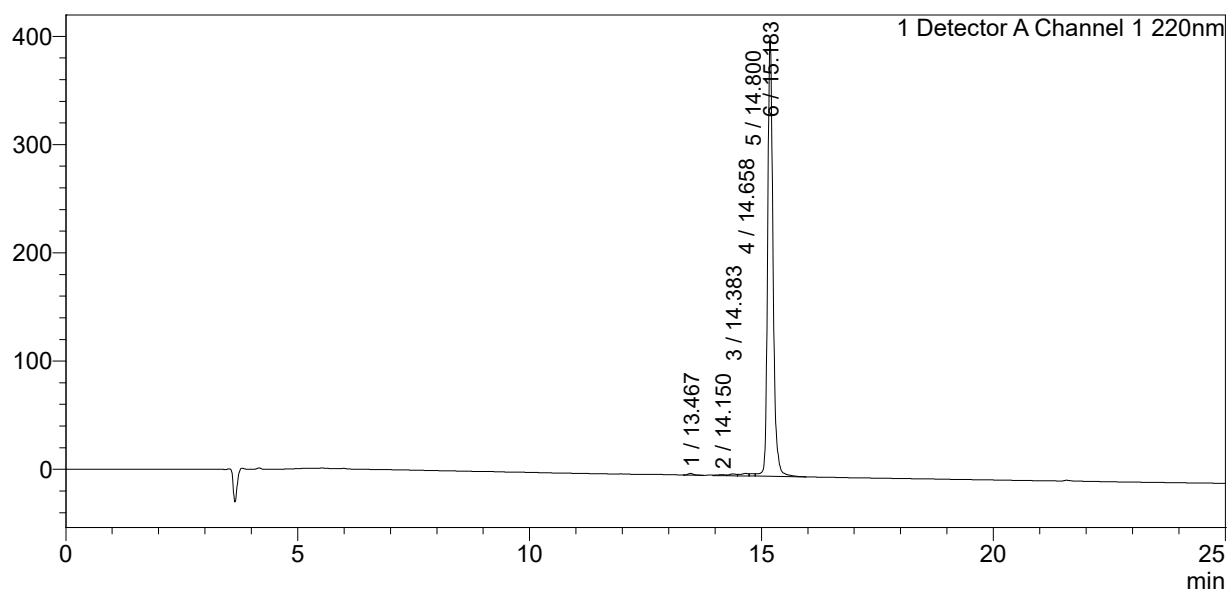

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.467	15111	1723	0.450
2	14.150	12295	1009	0.366
3	14.383	18576	1775	0.553
4	14.658	27935	2341	0.832
5	14.800	17492	2248	0.521
6	15.183	3265055	402306	97.277
Total		3356463	411401	100.000