

Sample Name :Substance P  
 Cat No. : RP10178  
 Lot No. : E0719322B  
 Time Processed :21:42:47  
 Month-Day-Year Processed :02/22/2022  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	15
25.00	Pumps	B.Conc	75
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
31.00	Pumps	B.Conc	5
31.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

mV

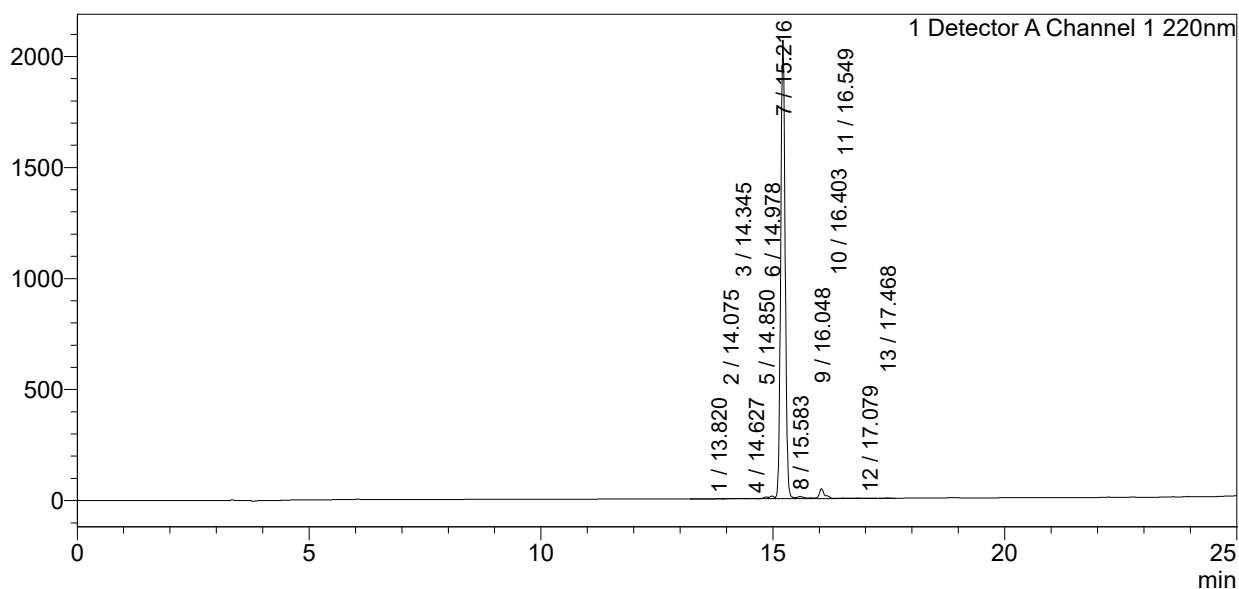

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.820	4323	200	0.030
2	14.075	1304	147	0.009
3	14.345	3621	340	0.025
4	14.627	8308	890	0.058
5	14.850	51636	7792	0.360
6	14.978	78994	12045	0.550
7	15.216	13703702	2065101	95.489
8	15.583	100935	9181	0.703
9	16.048	372842	44235	2.598
10	16.403	6401	854	0.045
11	16.549	5975	461	0.042
12	17.079	3488	152	0.024
13	17.468	9486	1364	0.066
Total		14351015	2142761	100.000