


Mass Spectrum

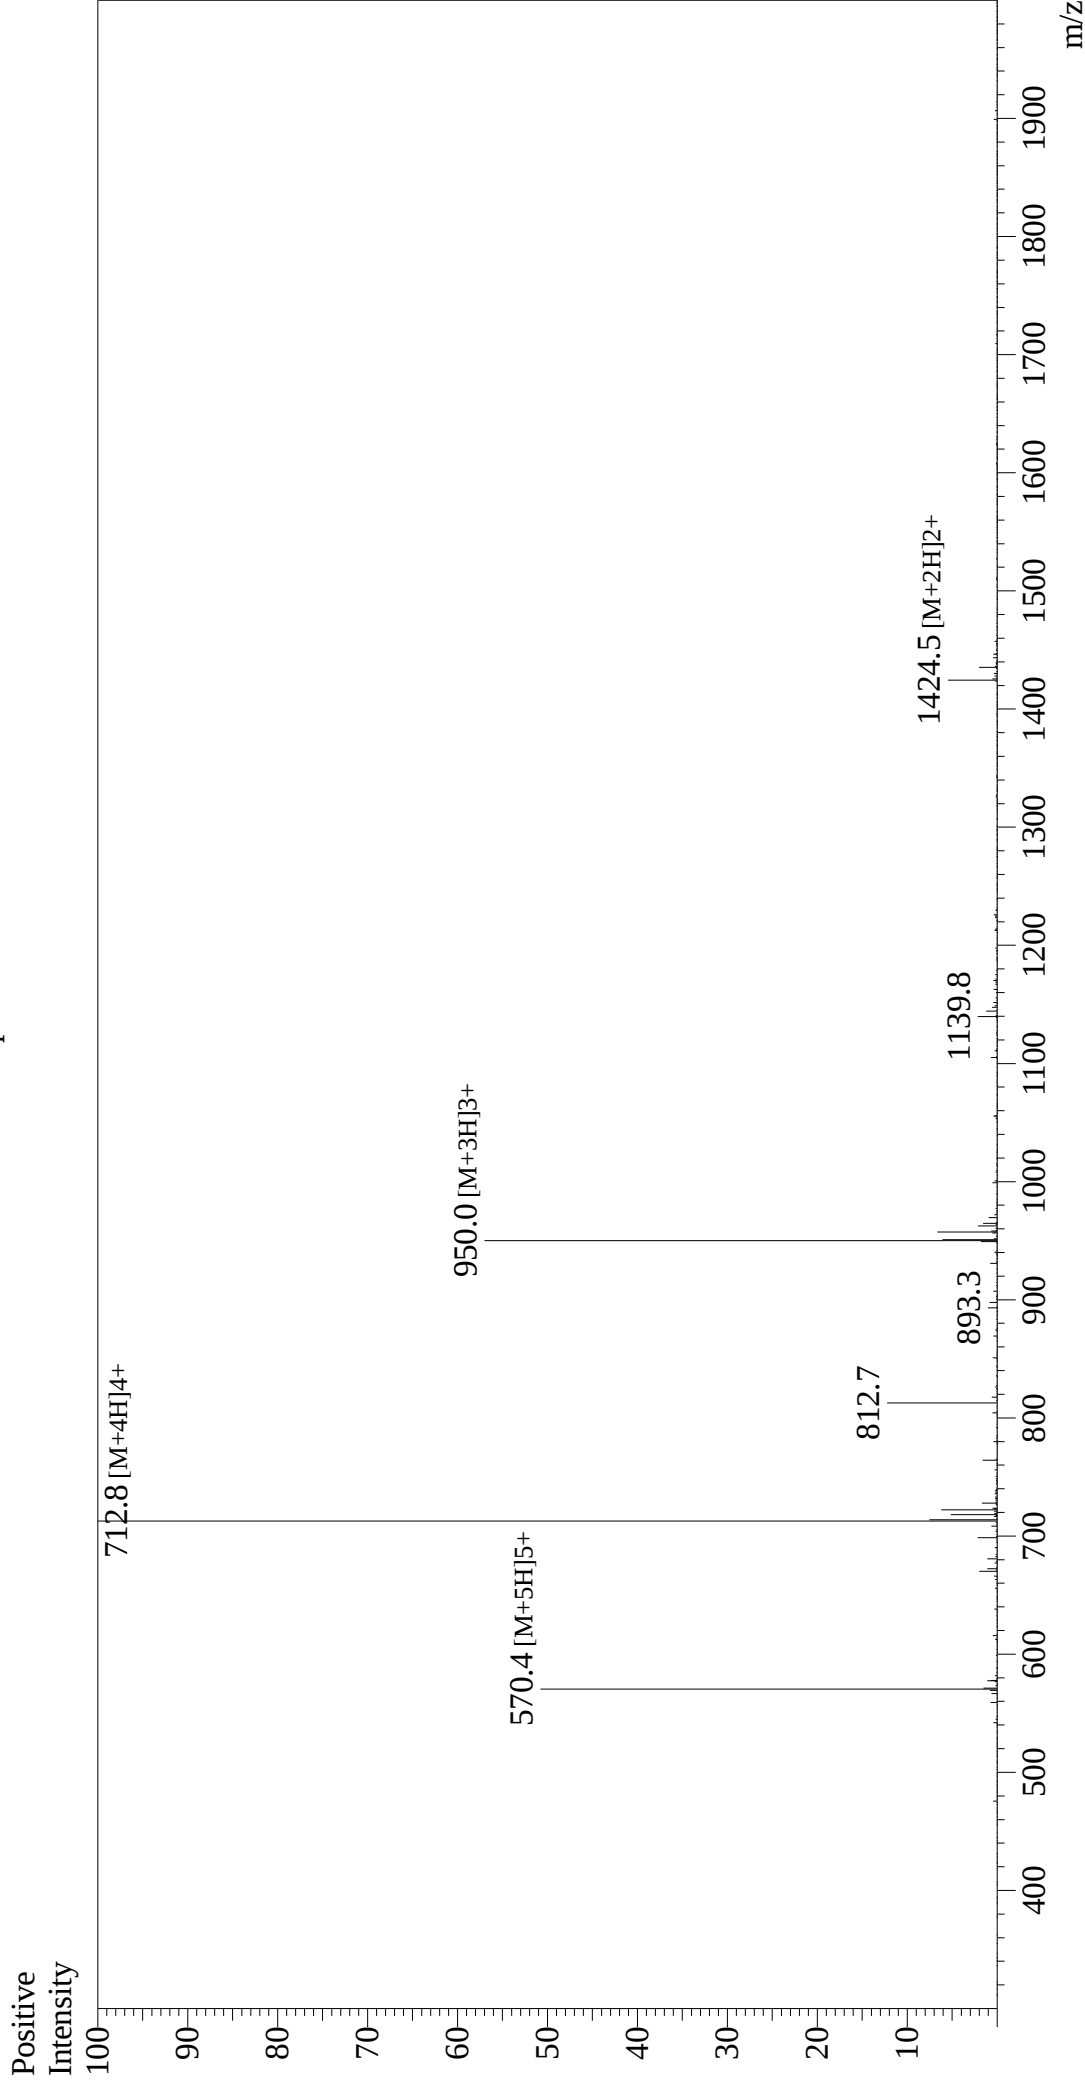

Sample Information

Month-Day Processed : 03/01/24
Time Processed : 17:18:06
Injection Volume : 0.2
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : E0775724B
Theoretical MW : 2847.50
Observed MW : 2847.2

Interface :ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment :ZJ22010150
Interface Bias :+4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH