


Sample Name :Glucagon-Like Peptide (GLP) II, human
Cat No. :RP10769
Lot No. :E0836725K
Time Processed :13:39:44
Month-Day-Year Processed :12/17/2025
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>
<Detector A>
Column :Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ20010139

<Chromatogram>

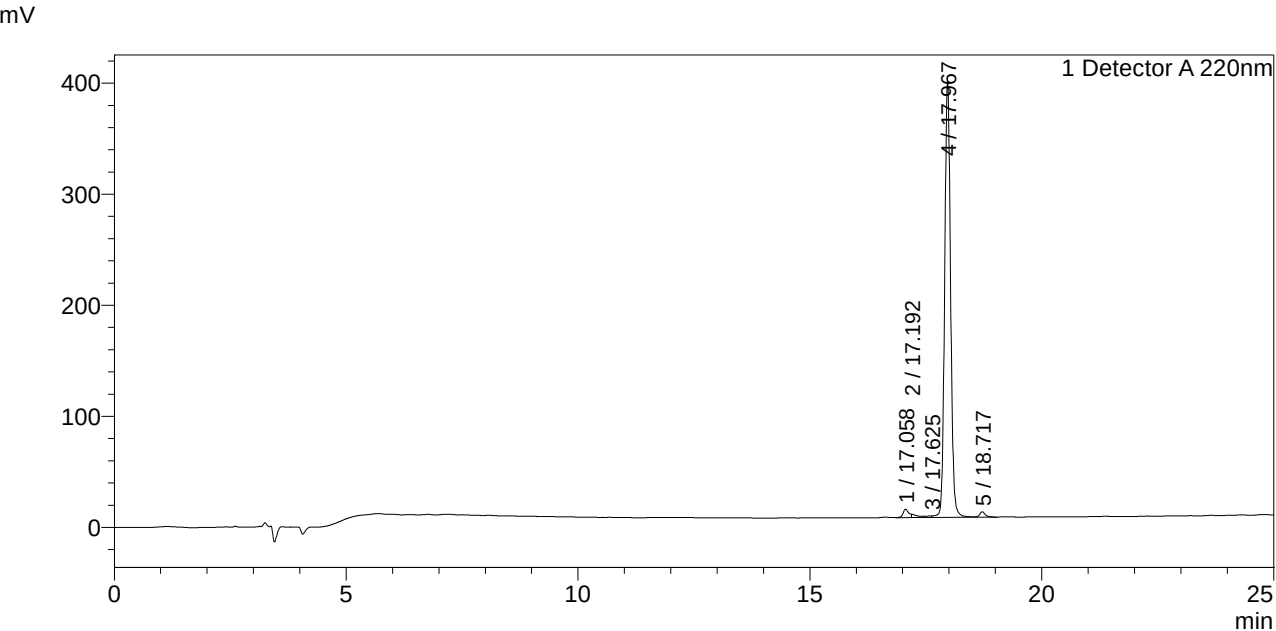

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.058	66540	7643	1.822
2	17.192	29095	3100	0.796
3	17.625	12711	1526	0.348
4	17.967	3499097	393243	95.788
5	18.717	45505	5104	1.246
Total		3652948	410616	100.000