


Mass Spectrum

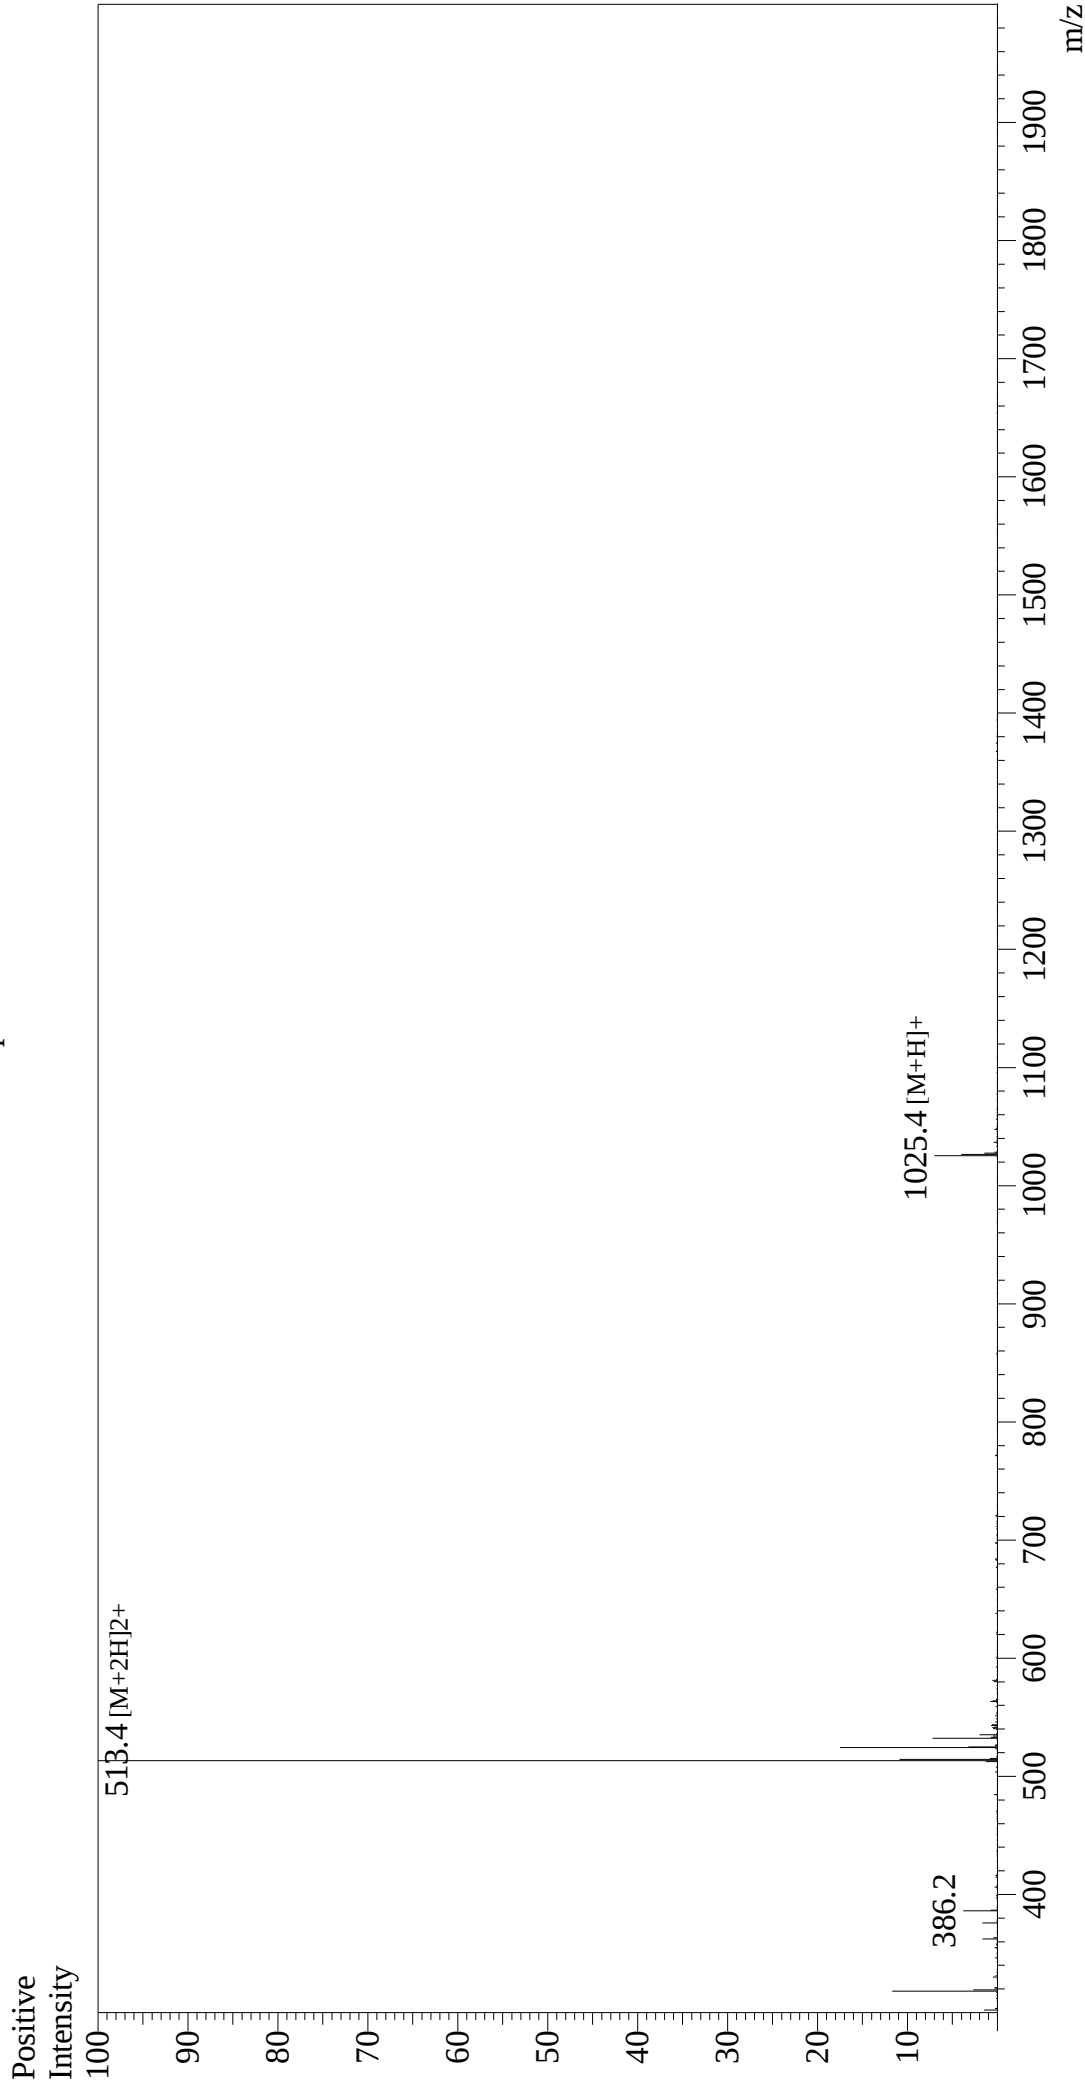

Sample Information

Month-Day Processed : 11/23/25

Time Processed : 10:23:24

Injection Volume : 0.3

Sample Name : RGD

Cat No. : RP20297

Lot No. : E0837625K

Theoretical MW : 1025.06

Observed MW : 1024.8

Interface : ESI

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment : ZJ21010035

Interface Bias : +4.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50% H₂O/50% MeOH