

Sample Name :Biotin-β-Amyloid (1-40)

Cat No. :RP30249

Lot No. :E1057326B

Time Processed :10:34:52

Month-Day-Year Processed :02/13/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPSN 30-300 30um, 4.6x250mm

<Chromatogram>

mV

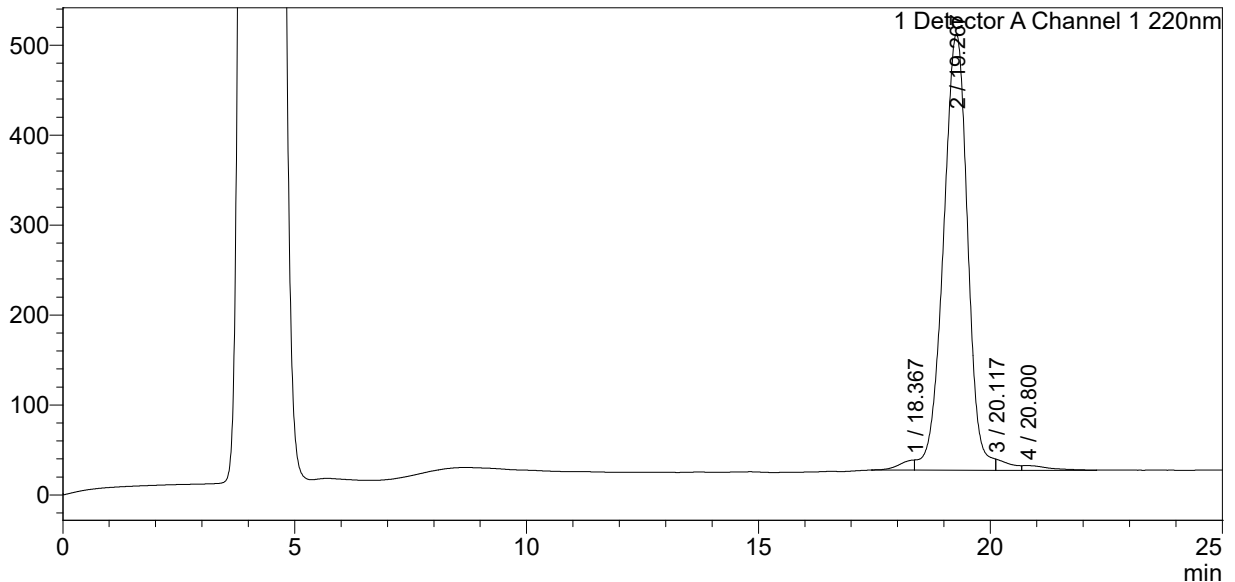

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.367	247535	11269	1.352
2	19.267	17573771	485376	95.975
3	20.117	263583	12442	1.439
4	20.800	225935	5178	1.234
Total		18310825	514264	100.000