


Mass Spectrum

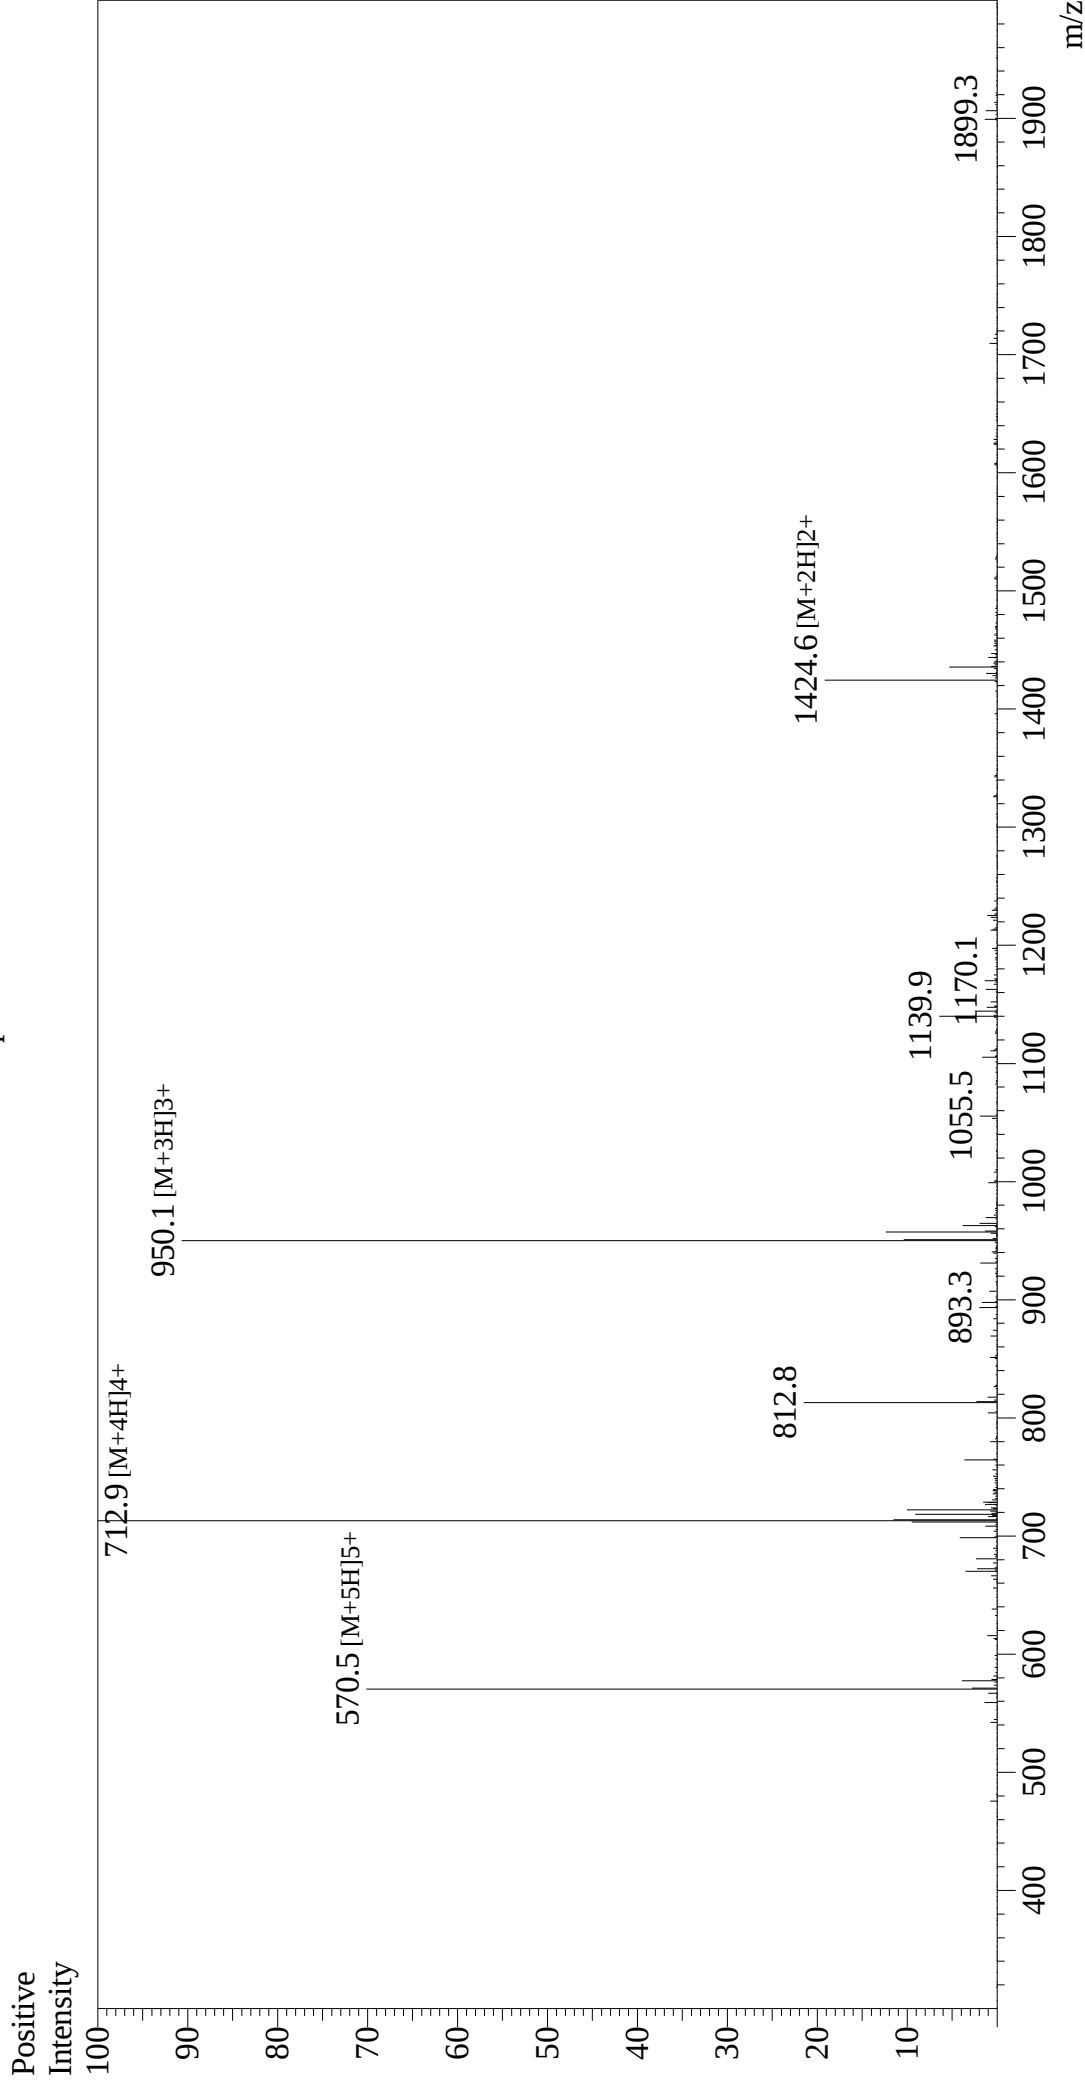

Sample Information

Month-Day Processed : 02/27/24
 Time Processed : 16:11:15
 Injection Volume : 0.3
 Sample Name : Melittin,honey bee
 Cat No. : RP20415
 Lot No. : E1066824B
 Theoretical MW:2847.50
 Observed MW : 2847.6

Interface

Nebulizing Gas Flow :1.5L/min
 CDL Temp :250
 Block Temp :200

Equipment

Interface Bias
 Drying Gas Flow
 T.Flow
 B.conc

:ZJ22010150

: +4.5 kV

:5 L/min

:0.2 ml/min

:50%H₂O/50%MeOH