

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat

Cat No. : RP11095

Lot No. : E1102422C

Time Processed :17:03:47

Month-Day-Year Processed :03/25/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	15
25.00	Pumps	B.Conc	75
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
31.00	Pumps	B.Conc	5
90.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010324

<Chromatogram>

mV

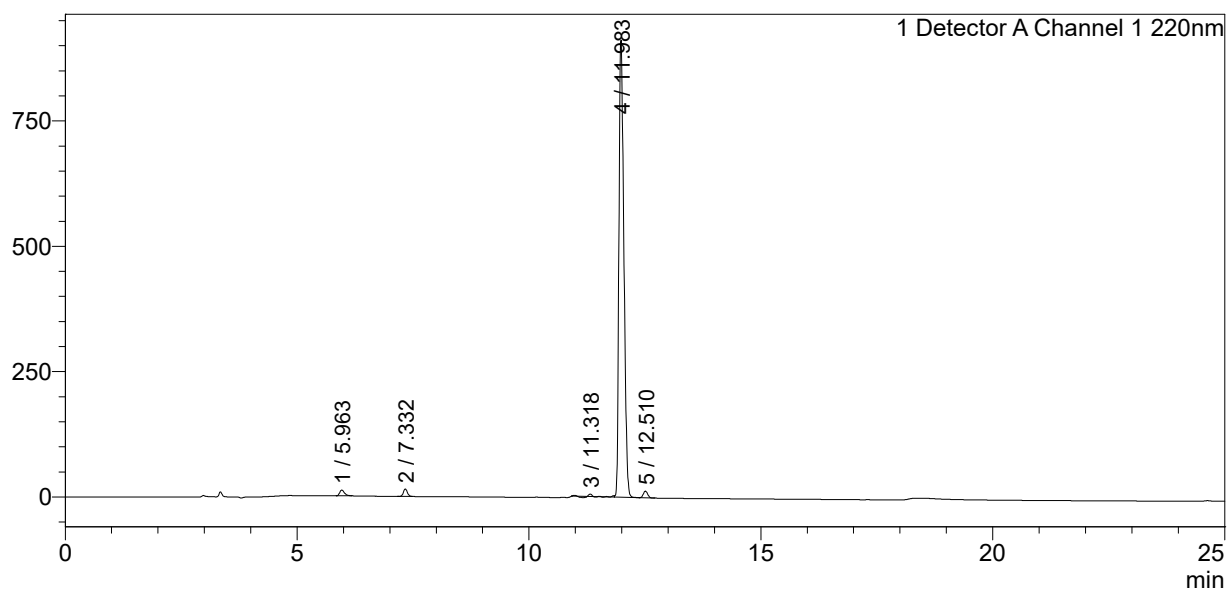

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.963	80928	11414	1.155
2	7.332	88287	14908	1.260
3	11.318	25225	5133	0.360
4	11.983	6723321	912097	95.950
5	12.510	89358	13696	1.275
Total		7007119	957247	100.000