


Sample Name :Glucagon-Like Peptide (GLP) II, human
Cat No. :RP10769
Lot No. :E1186126C
Time Processed :15:45:03
Month-Day-Year Processed :04/07/2026
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	

<<Column Performance>>
<Detector A>
Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ17010509

<Chromatogram>

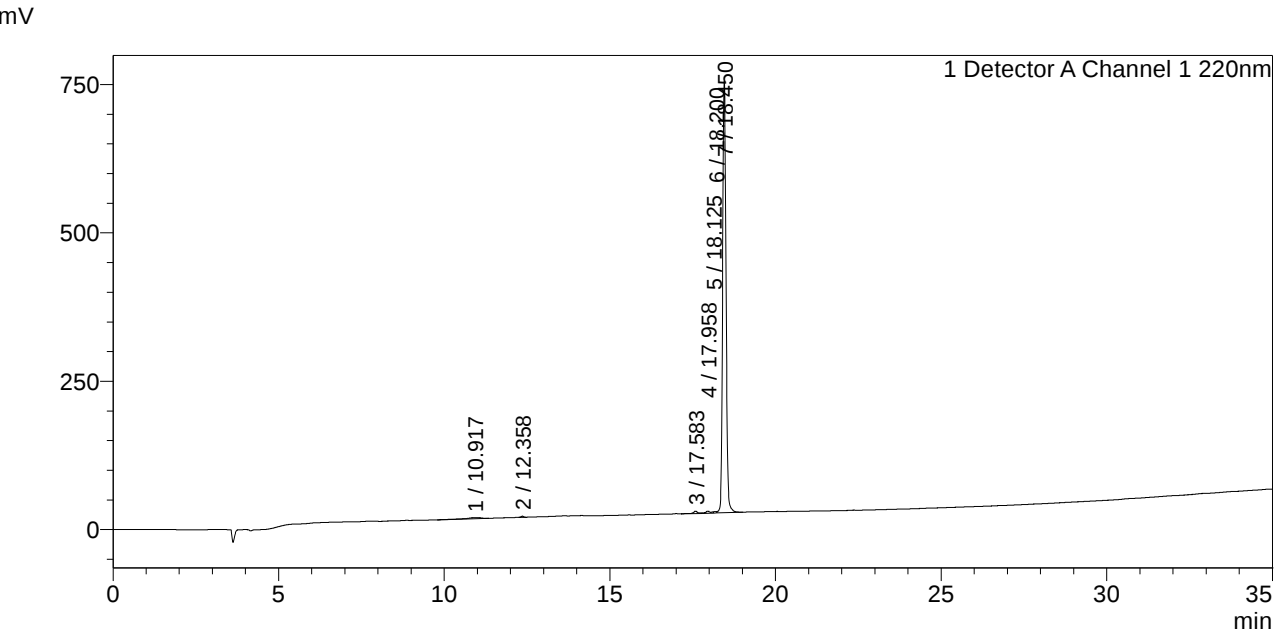

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.917	57644	1686	1.077
2	12.358	9861	1921	0.184
3	17.583	40287	4060	0.752
4	17.958	28705	3553	0.536
5	18.125	9150	2142	0.171
6	18.200	16117	2648	0.301
7	18.450	5192290	727341	96.979
Total		5354054	743350	100.000