
Mass Spectrum

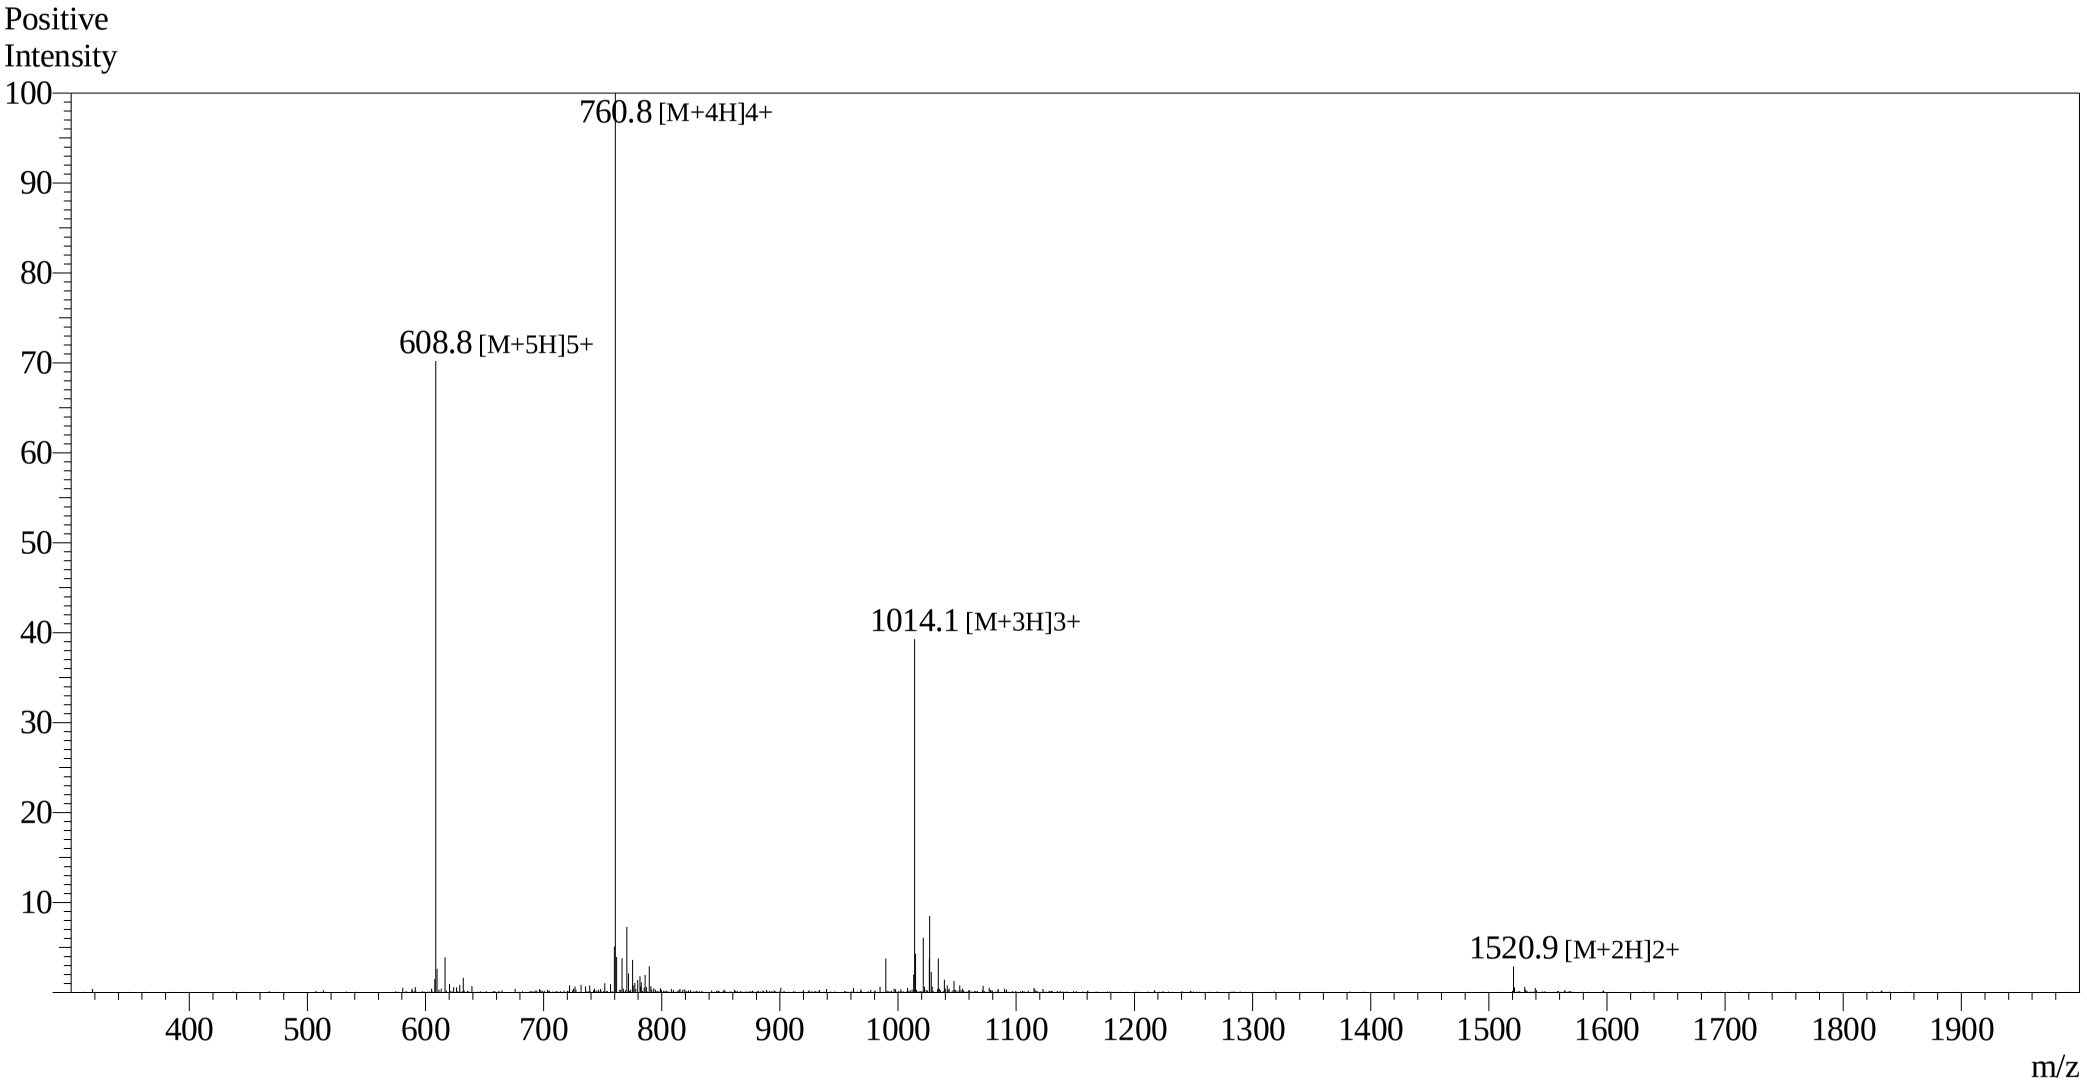

Sample Information
Month-Day Processed : 02/28/26
Time Processed : 17:05:30
Injection Volume : 0.4
Sample Name : Secretin, human
Cat No. :RP10249
Lot No. :E1245226B
Theoretical MW : 3039.50
Observed MW : 3039.2

Interface :ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH