


Mass Spectrum

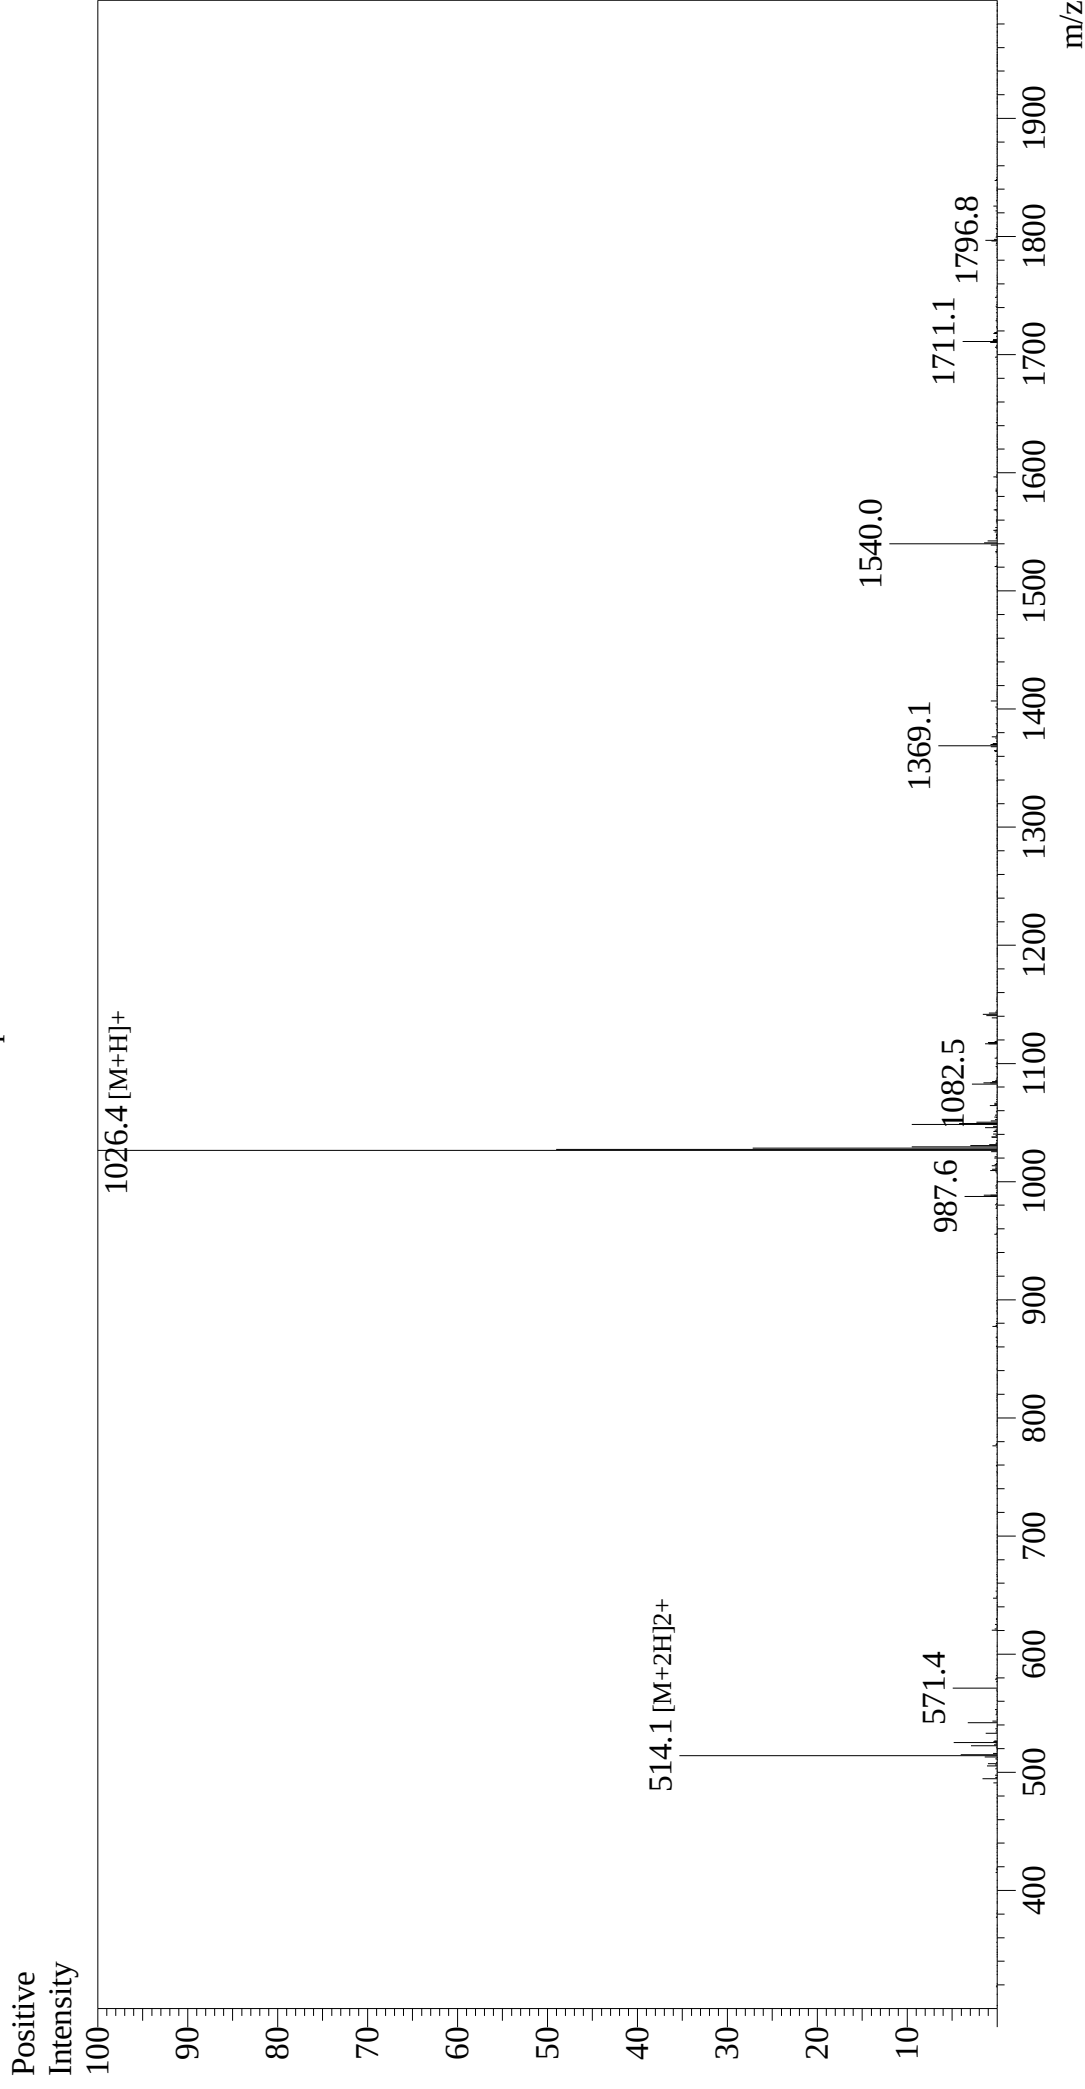

Sample Information

Month-Day Processed :	02/10/26	Equipment	:ZJ22010150
Time Processed :	21:40:55	Interface Bias	: +4.5 kV
Injection Volume :	0.3	Drying Gas Flow	:5 L/min
Sample Name :	Influenza A NP(366-374) Strain A/PR/8/35	T.Flow	:0.2 ml/min
Cat No. : RP20267		B.conc	:50%H2O/50%MeOH
Lot No. : E1264826B			
Theoretical MW: 1026.12			
Observed MW : 1025.4			