

Sample Name: Biotin- β -Amyloid (1-40)
 Cat No. : RP30249
 Lot No. : E1280426B
 Time Processed :9:43:27
 Month-Day-Year Processed :03/05/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPS 10-300 10um, 4.6x250mm

<Chromatogram>

mV

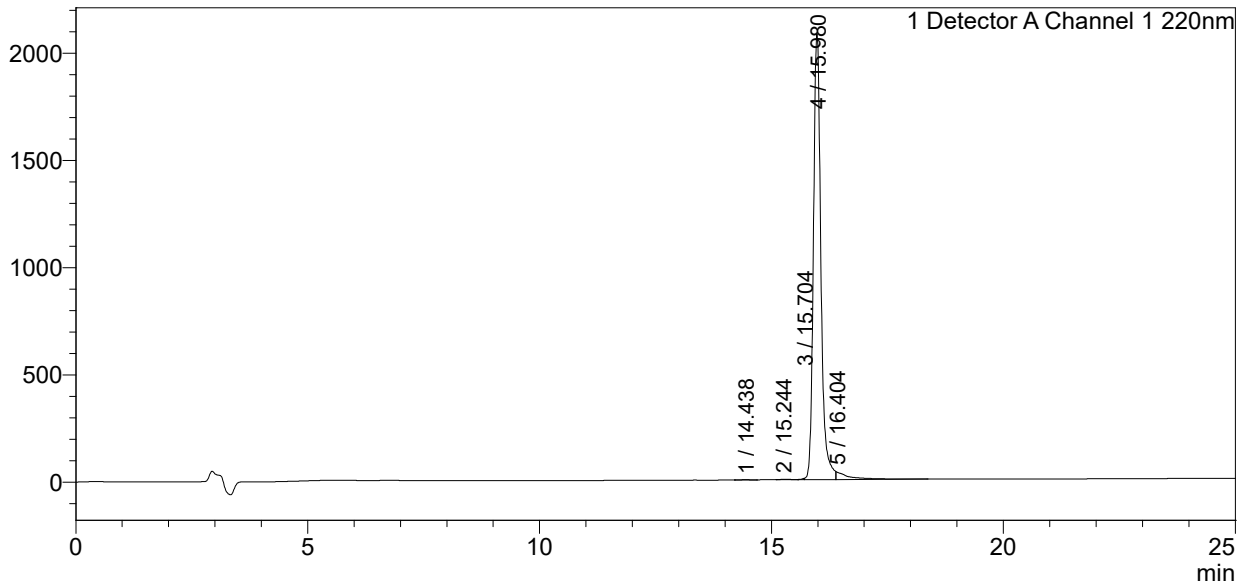

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.438	9116	1275	0.038
2	15.244	27897	1801	0.116
3	15.704	24402	5892	0.101
4	15.980	23330975	2080025	96.797
5	16.404	710689	35728	2.949
Total		24103079	2124722	100.000