

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E1336323E
Time Processed :6:19:34
Month-Day-Year Processed :06/18/2023
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: GR11010440

<Chromatogram>

mV

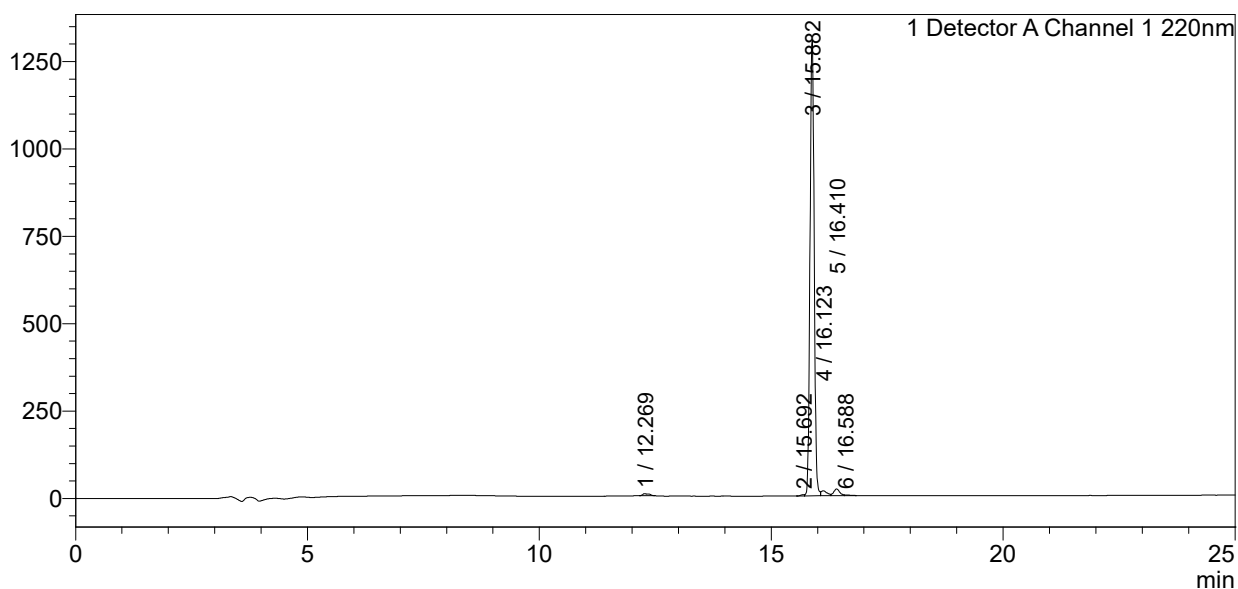

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.269	58275	5890	0.687
2	15.692	19145	3661	0.226
3	15.882	8097796	1303237	95.418
4	16.123	125065	14372	1.474
5	16.410	172327	19420	2.031
6	16.588	14021	2007	0.165
Total		8486628	1348587	100.000