


Mass Spectrum

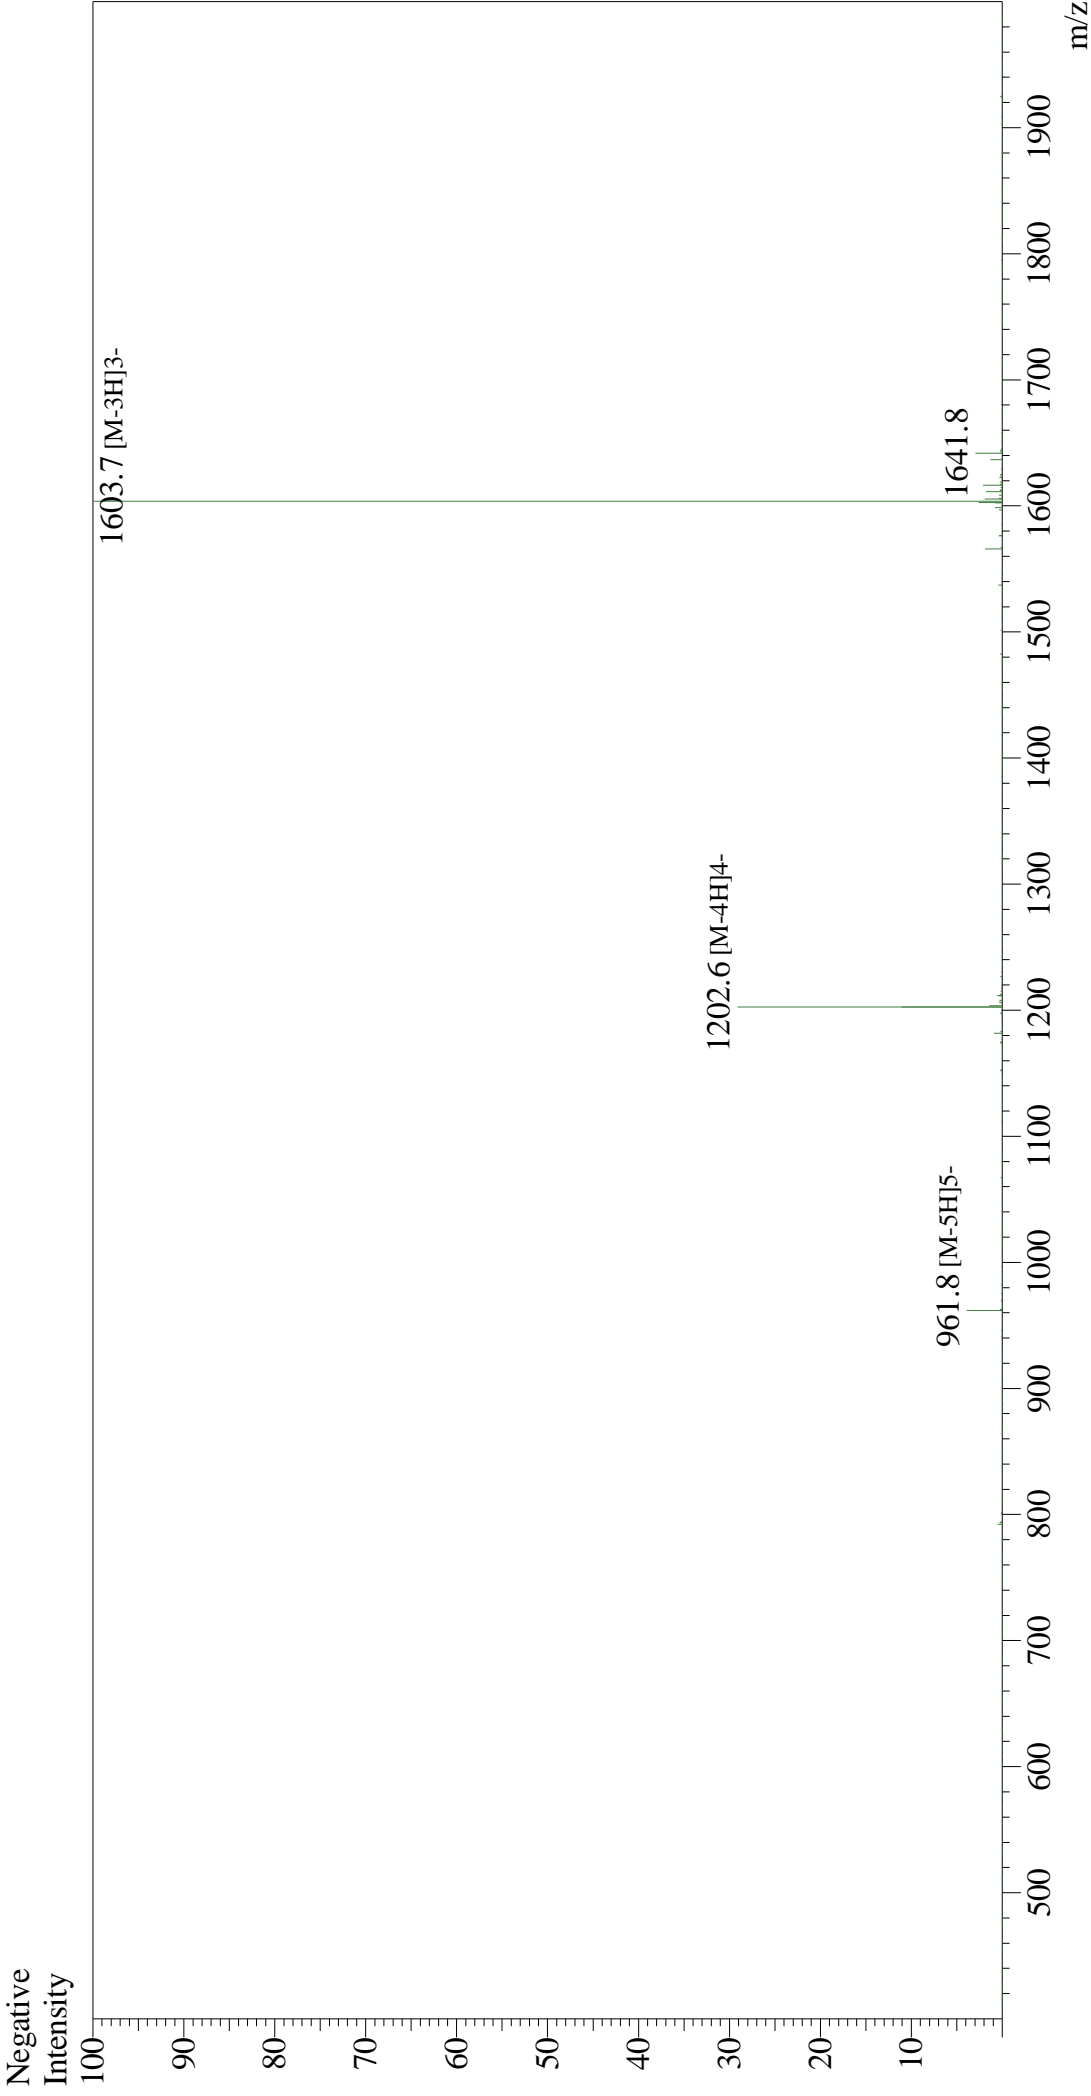

Sample Information

Month-Day Processed : 06/06/25  
Time Processed : 6:31:23 PM  
Injection Volume : 0.6  
Sample Name : Glu19-Tirzepatide  
Cat No. : RP30874  
Lot No. : E1363725E  
Theoretical MW: 4814.36  
Observed MW : 4814.1

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : ZJ22010150  
Interface Bias : -3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% H<sub>2</sub>O/50% MeOH