

Sample Name :Glu24-Tirzepatide
Cat No. : RP30875
Lot No. : E1364525E
Time Processed :17:52:25
Month-Day-Year Processed :06/07/2025
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ17010506

<Chromatogram>

mV

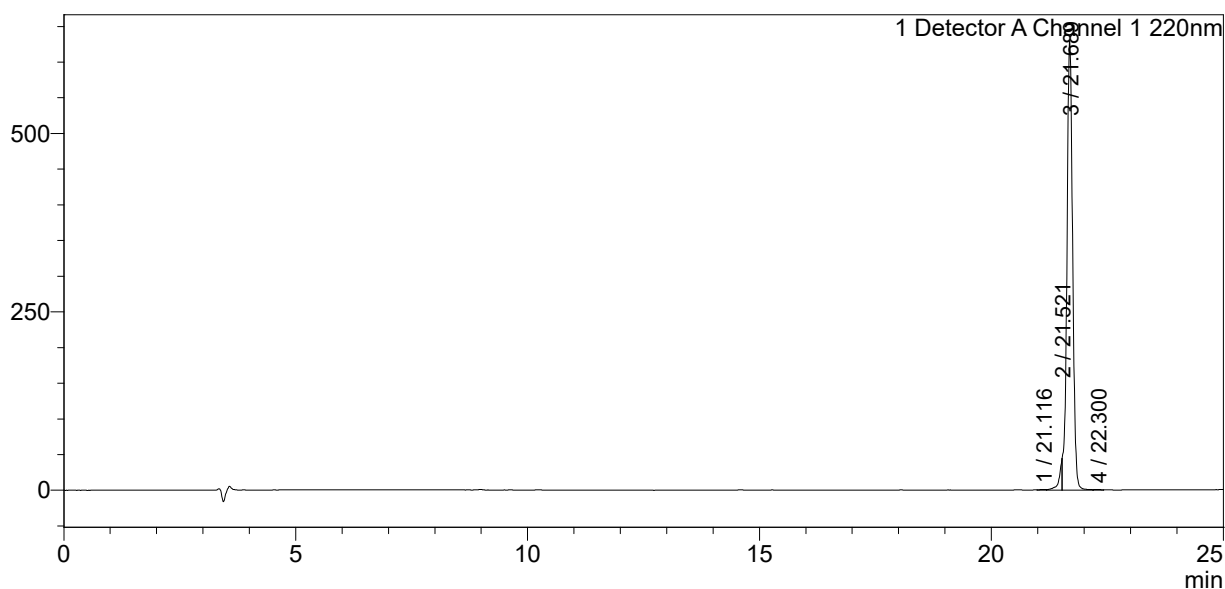

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.116	9248	984	0.165
2	21.521	190738	41140	3.396
3	21.689	5407199	630002	96.284
4	22.300	8696	835	0.155
Total		5615881	672961	100.000