


Mass Spectrum

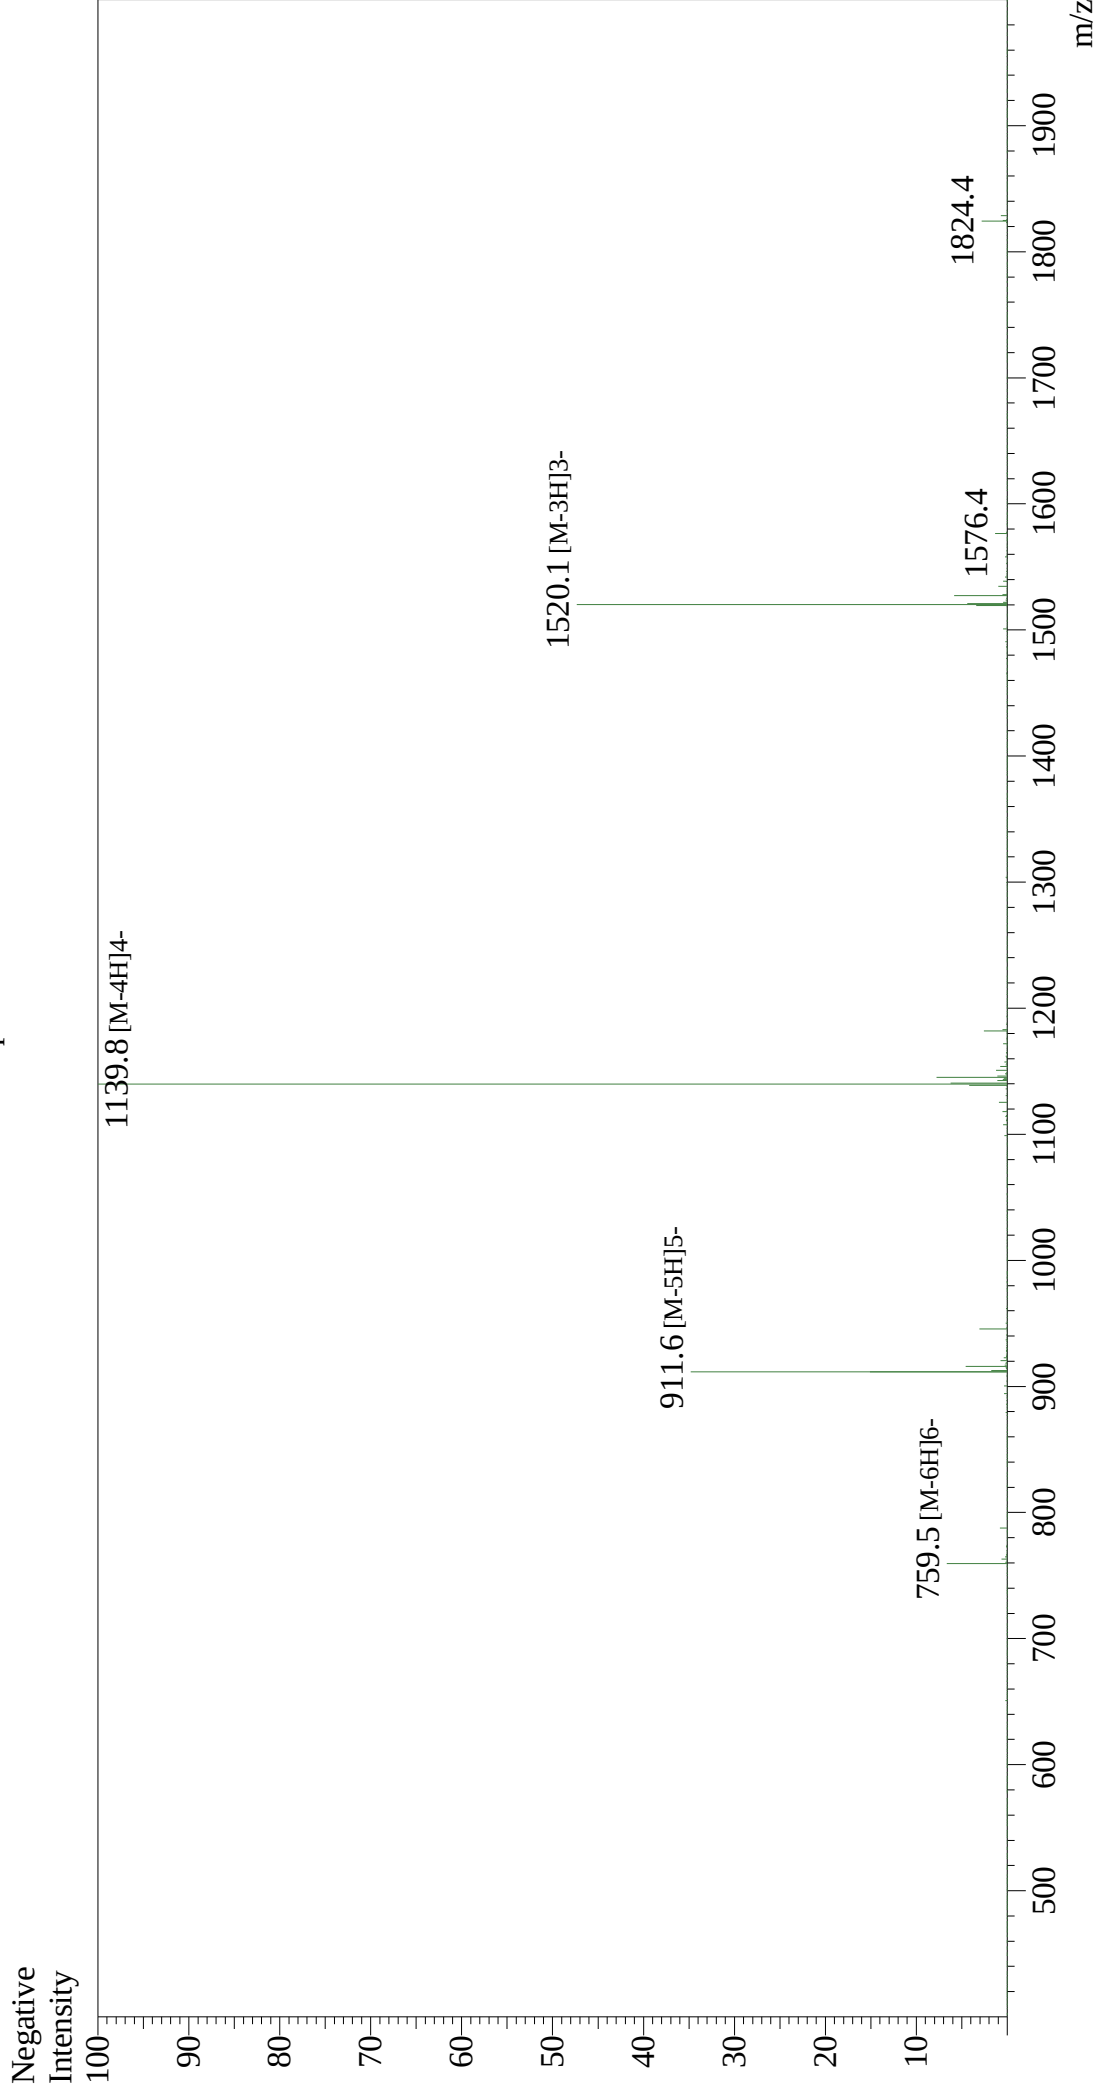

Sample Information

Month-Day Processed : 06/10/25
 Time Processed : 15:29:28
 Injection Volume : 0.8

Sample Name : [D-SER]33-Mazdutide

Cat No. : RP30899

Lot No. : E1401425E

Theoretical MW : 4563.14

Observed MW : 4563.2

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ22010150
 Interface Bias : -3.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH