


Mass Spectrum

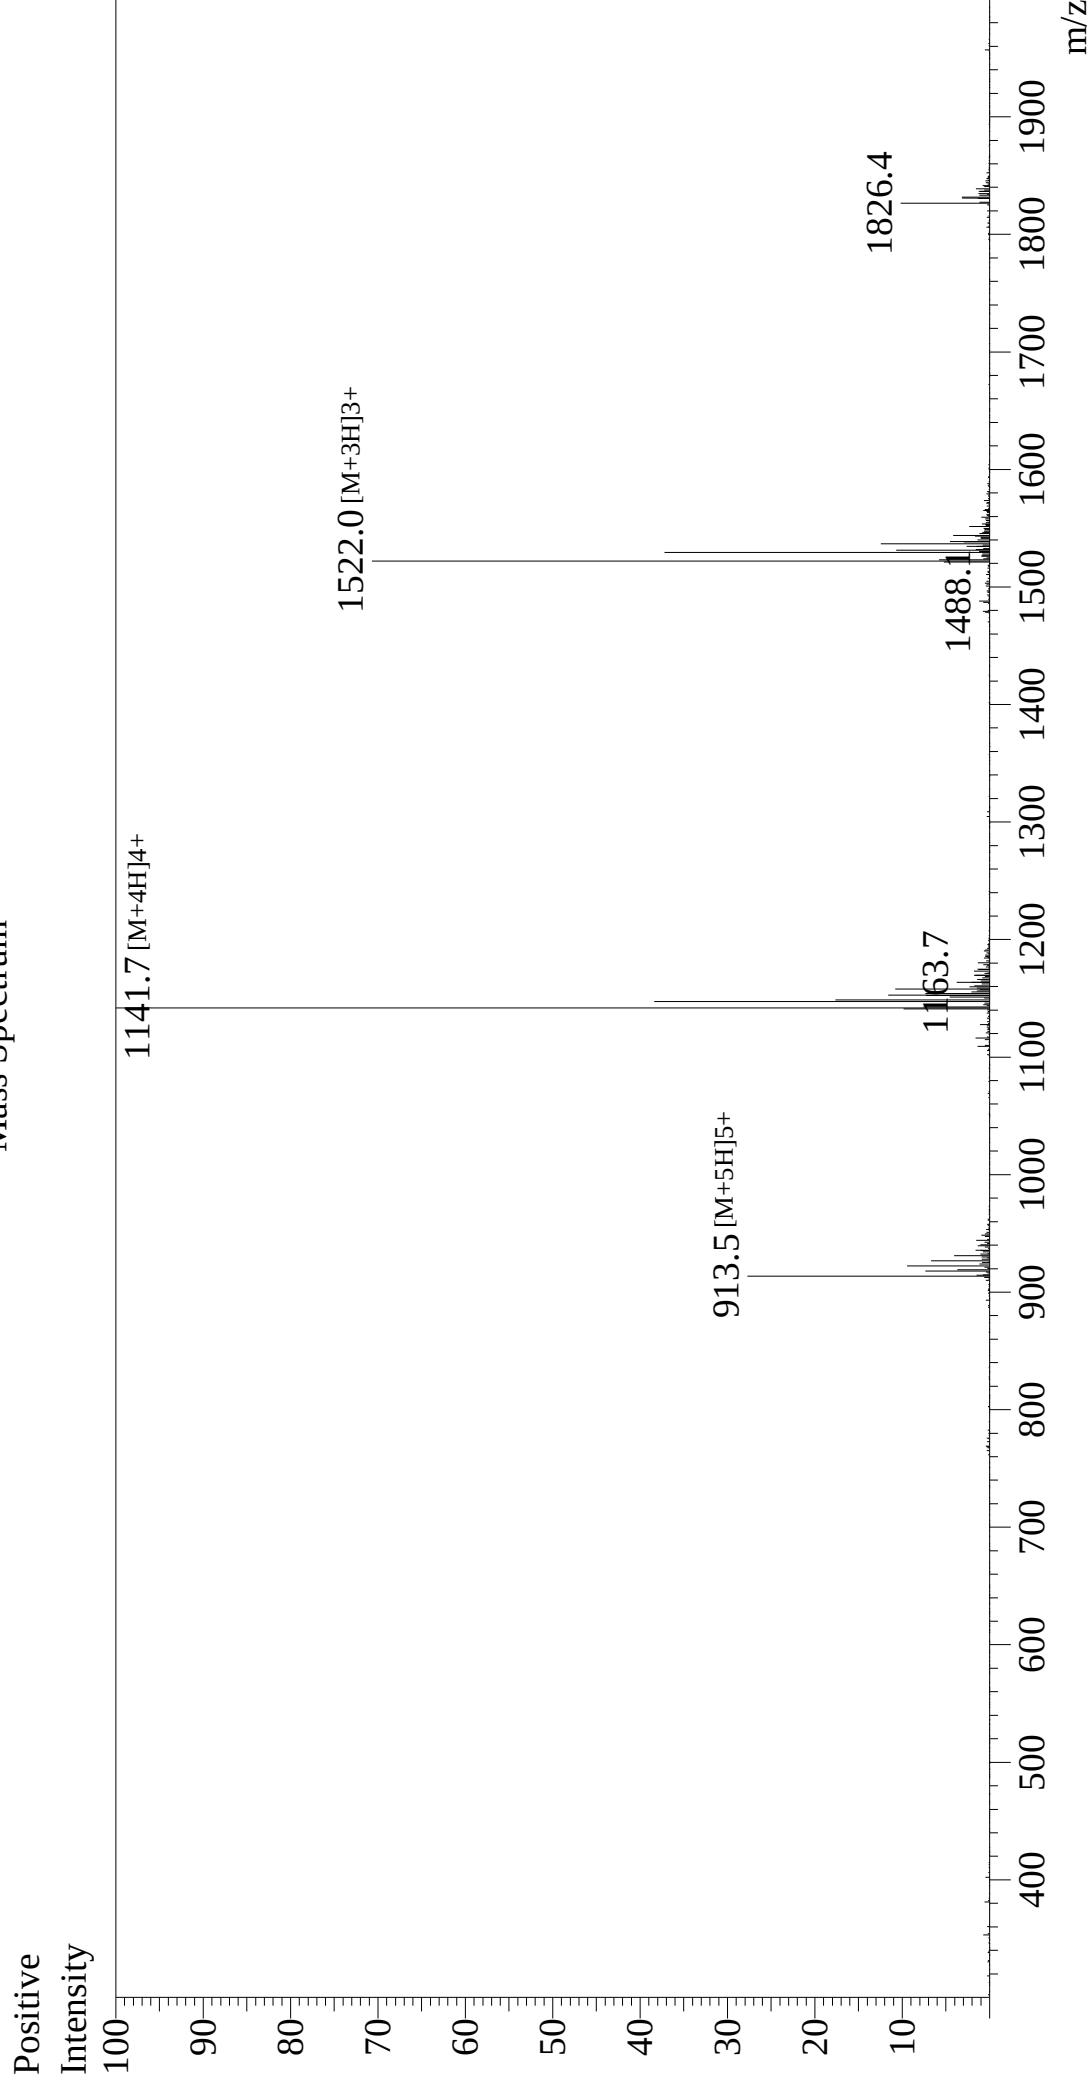

Sample Information

Month-Day Processed : 06/07/25
 Time Processed : 15:44:59
 Injection Volume : 0.4
 Sample Name : [D-GLU]16-Mazdutide
 Cat No. : RP30900
 Lot No. : E1403125E
 Theoretical MW : 4563.14
 Observed MW : 4562.8

Interface :ESI

Nebulizing Gas Flow :1.5L/min
 CDL Temp :250
 Block Temp :200

Equipment

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow :5 L/min
 T.Flow :0.2 ml/min
 B.conc :50%H₂O/50%MeOH