


# Mass Spectrum

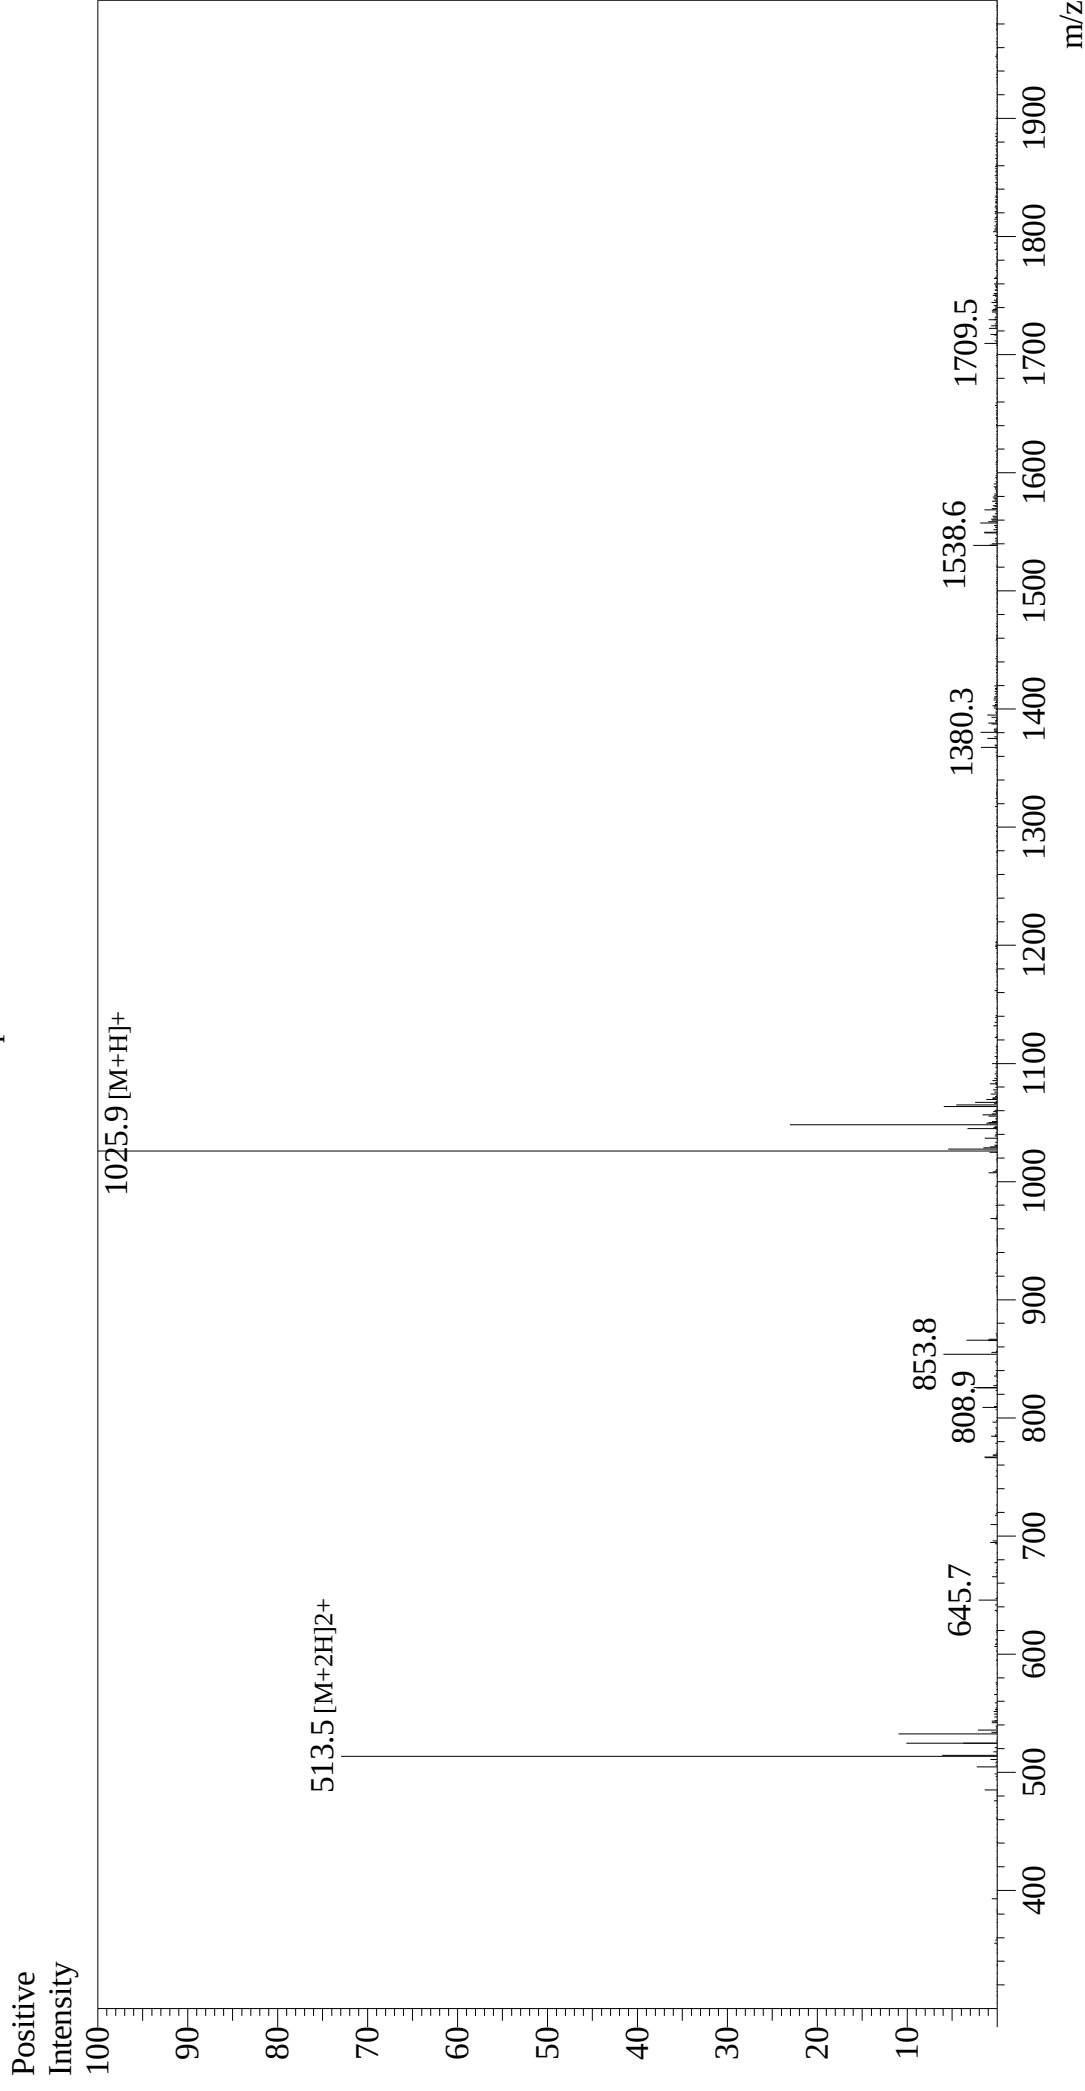

## Sample Information

Month-Day Processed : 06/02/23  
 Time Processed : 20:33:13  
 Injection Volume : 0.1  
 Sample Name : RGD  
 Cat No. : RP20297  
 Lot No. : E1496223E  
 Theoretical MW:1025.06  
 Observed MW : 1024.9

Interface :ESI  
 Nebulizing Gas Flow :1.5L/min  
 CDL Temp :250  
 Block Temp :200  
 Equipment :ZJ22010150  
 Interface Bias :+4.5 kV  
 Drying Gas Flow :5 L/min  
 T.Flow :0.2 ml/min  
 B.conc :50%H2O/50%MeOH