

Sample Name :Influenza A NP(366-374) Strain A/PR/8/35
Cat No. : RP20267
Lot No. : E1672026B

Time Processed : 2:10:10
Month-Day-Year Processed :02/14/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
Equipment:ZJ17010507

<Chromatogram>

mV

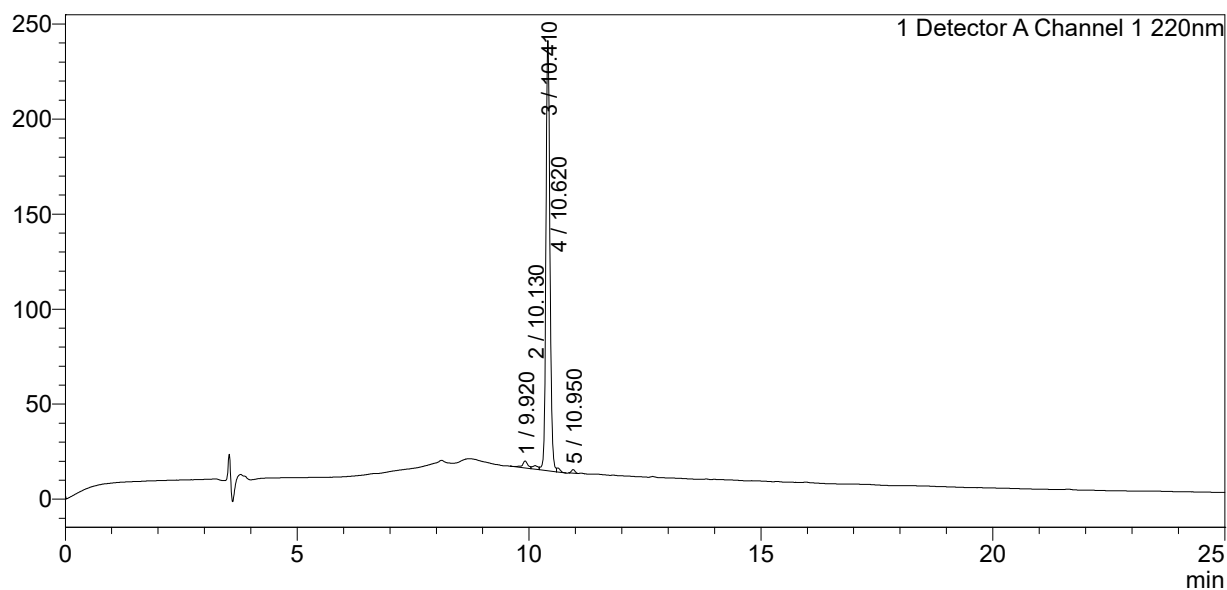

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.920	31040	3700	2.164
2	10.130	16398	1920	1.143
3	10.410	1365320	226419	95.174
4	10.620	11896	2165	0.829
5	10.950	9903	1869	0.690
Total		1434557	236073	100.000