


Mass Spectrum

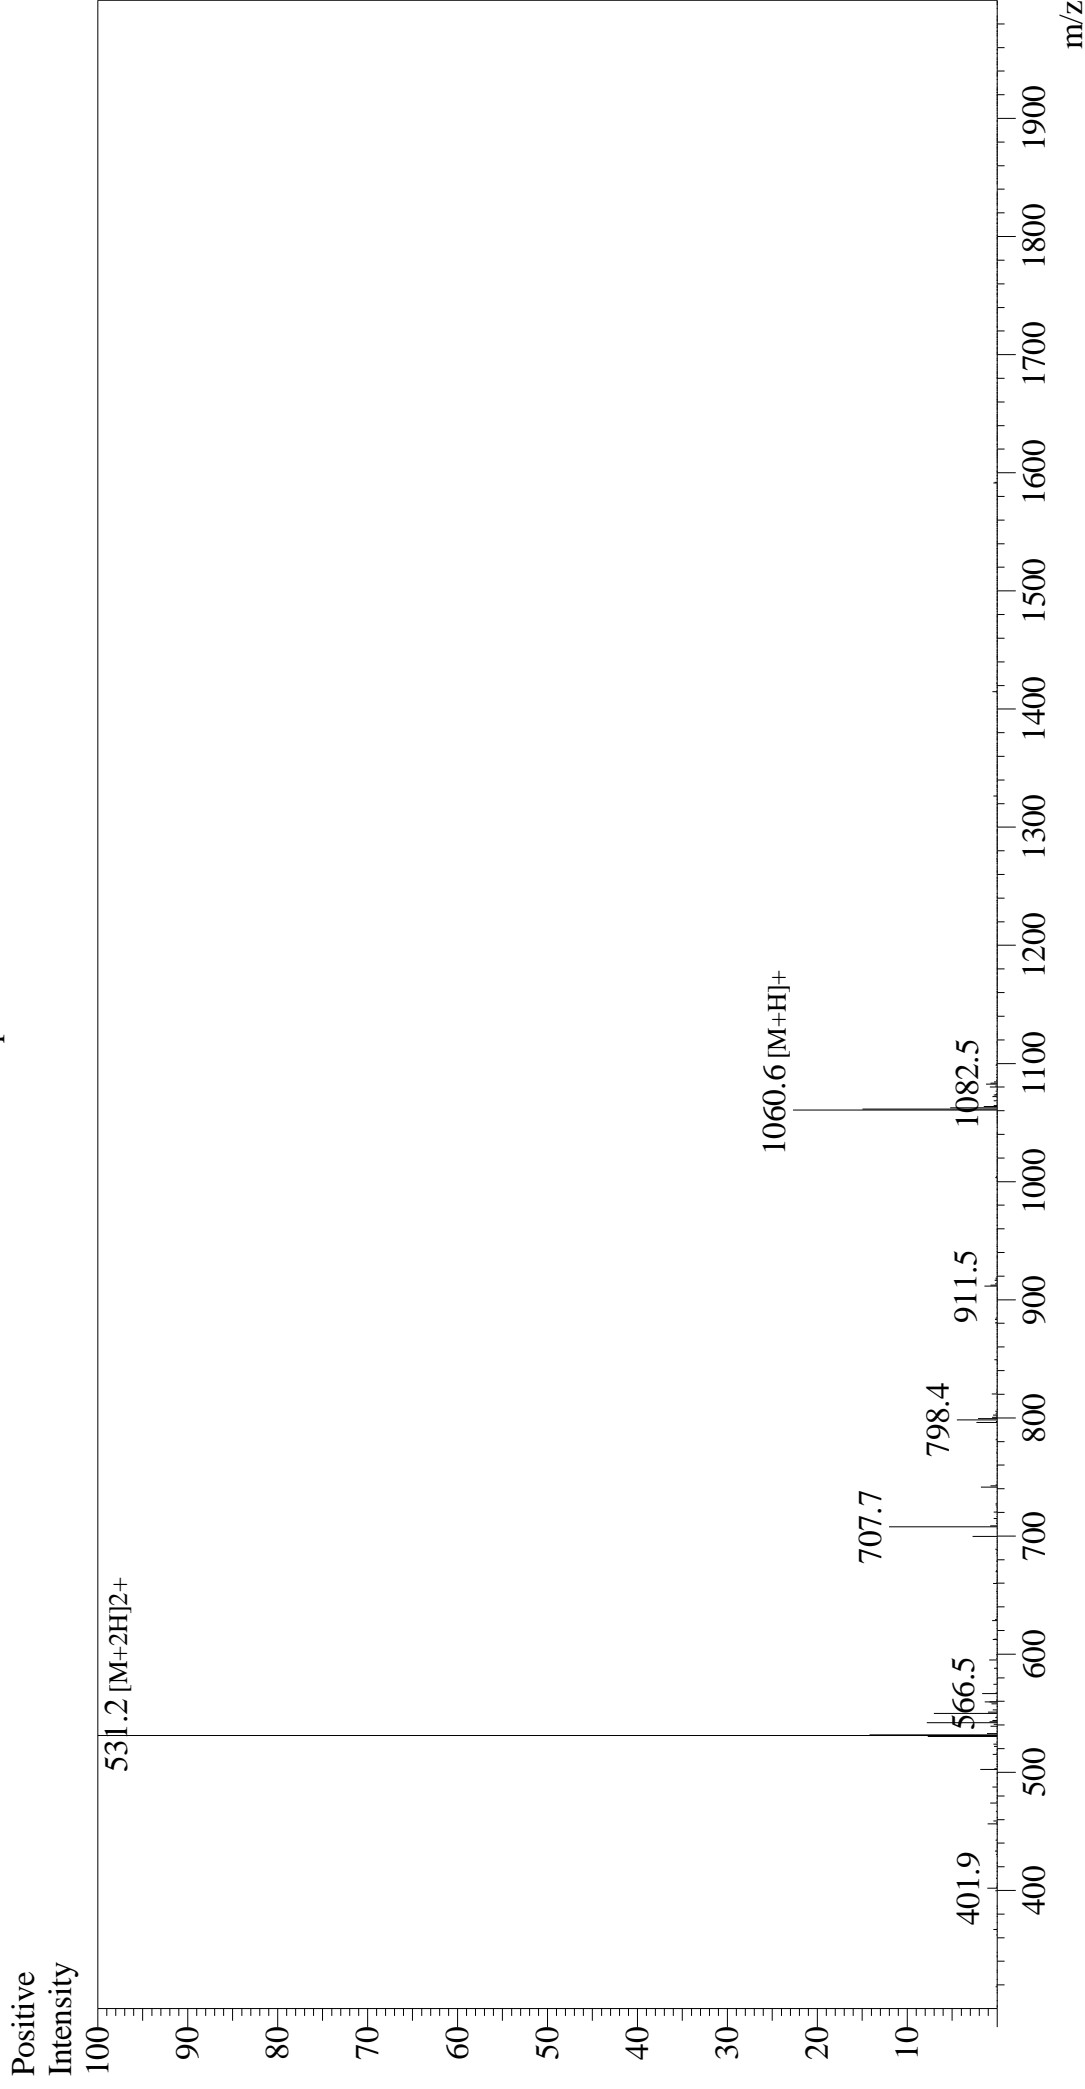

Sample Information

Month-Day Processed :	05/12/22	Equipment	: GK11010007
Time Processed :	19:57:10	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	:5 L/min
Sample Name :	β-Amyloid (25-35)	T.Flow	:0.2 ml/min
Cat No. :	RP10008	B.conc	:50%H2O/50%MeOH
Lot No. :	E1881322E		
Theoretical MW :	1060.27		
Observed MW :	1060.4		