

Sample Name: Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E2201625E
Time Processed :9:34:00
Month-Day-Year Processed :05/23/2025


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>
<Detector A>
Column :Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ23010112

<Chromatogram>

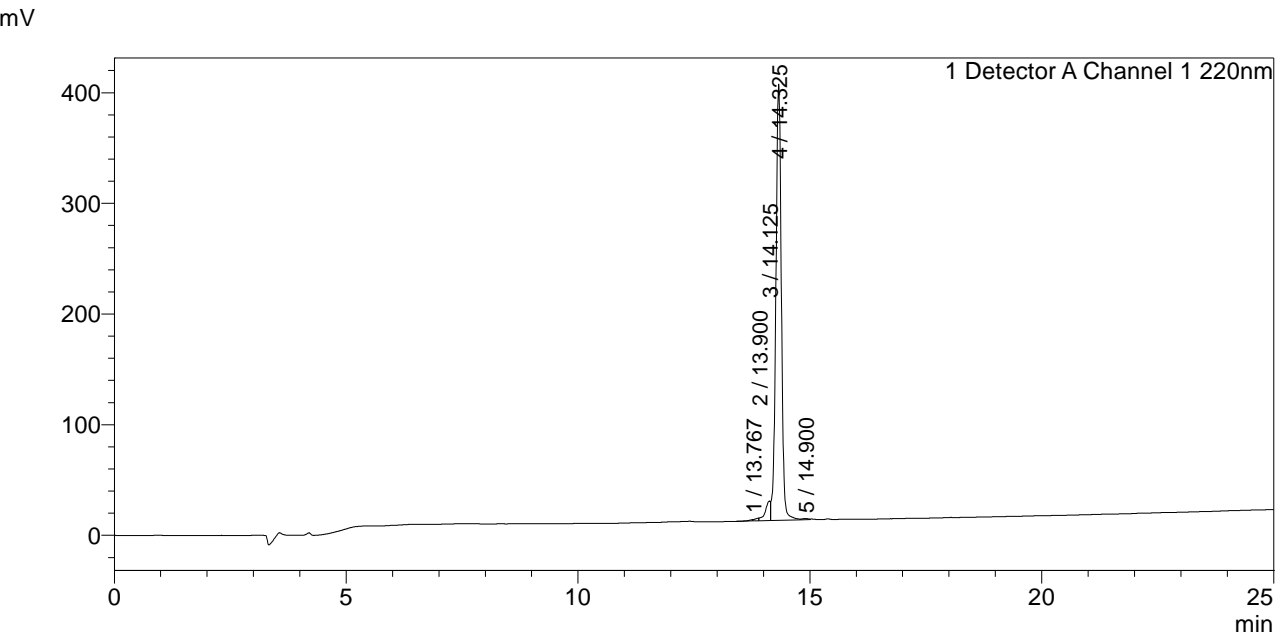

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.767	7263	1199	0.214
2	13.900	14577	2489	0.429
3	14.125	131525	17518	3.872
4	14.325	3233264	394474	95.186
5	14.900	10157	1094	0.299
Total		3396786	416775	100.000