


Mass Spectrum

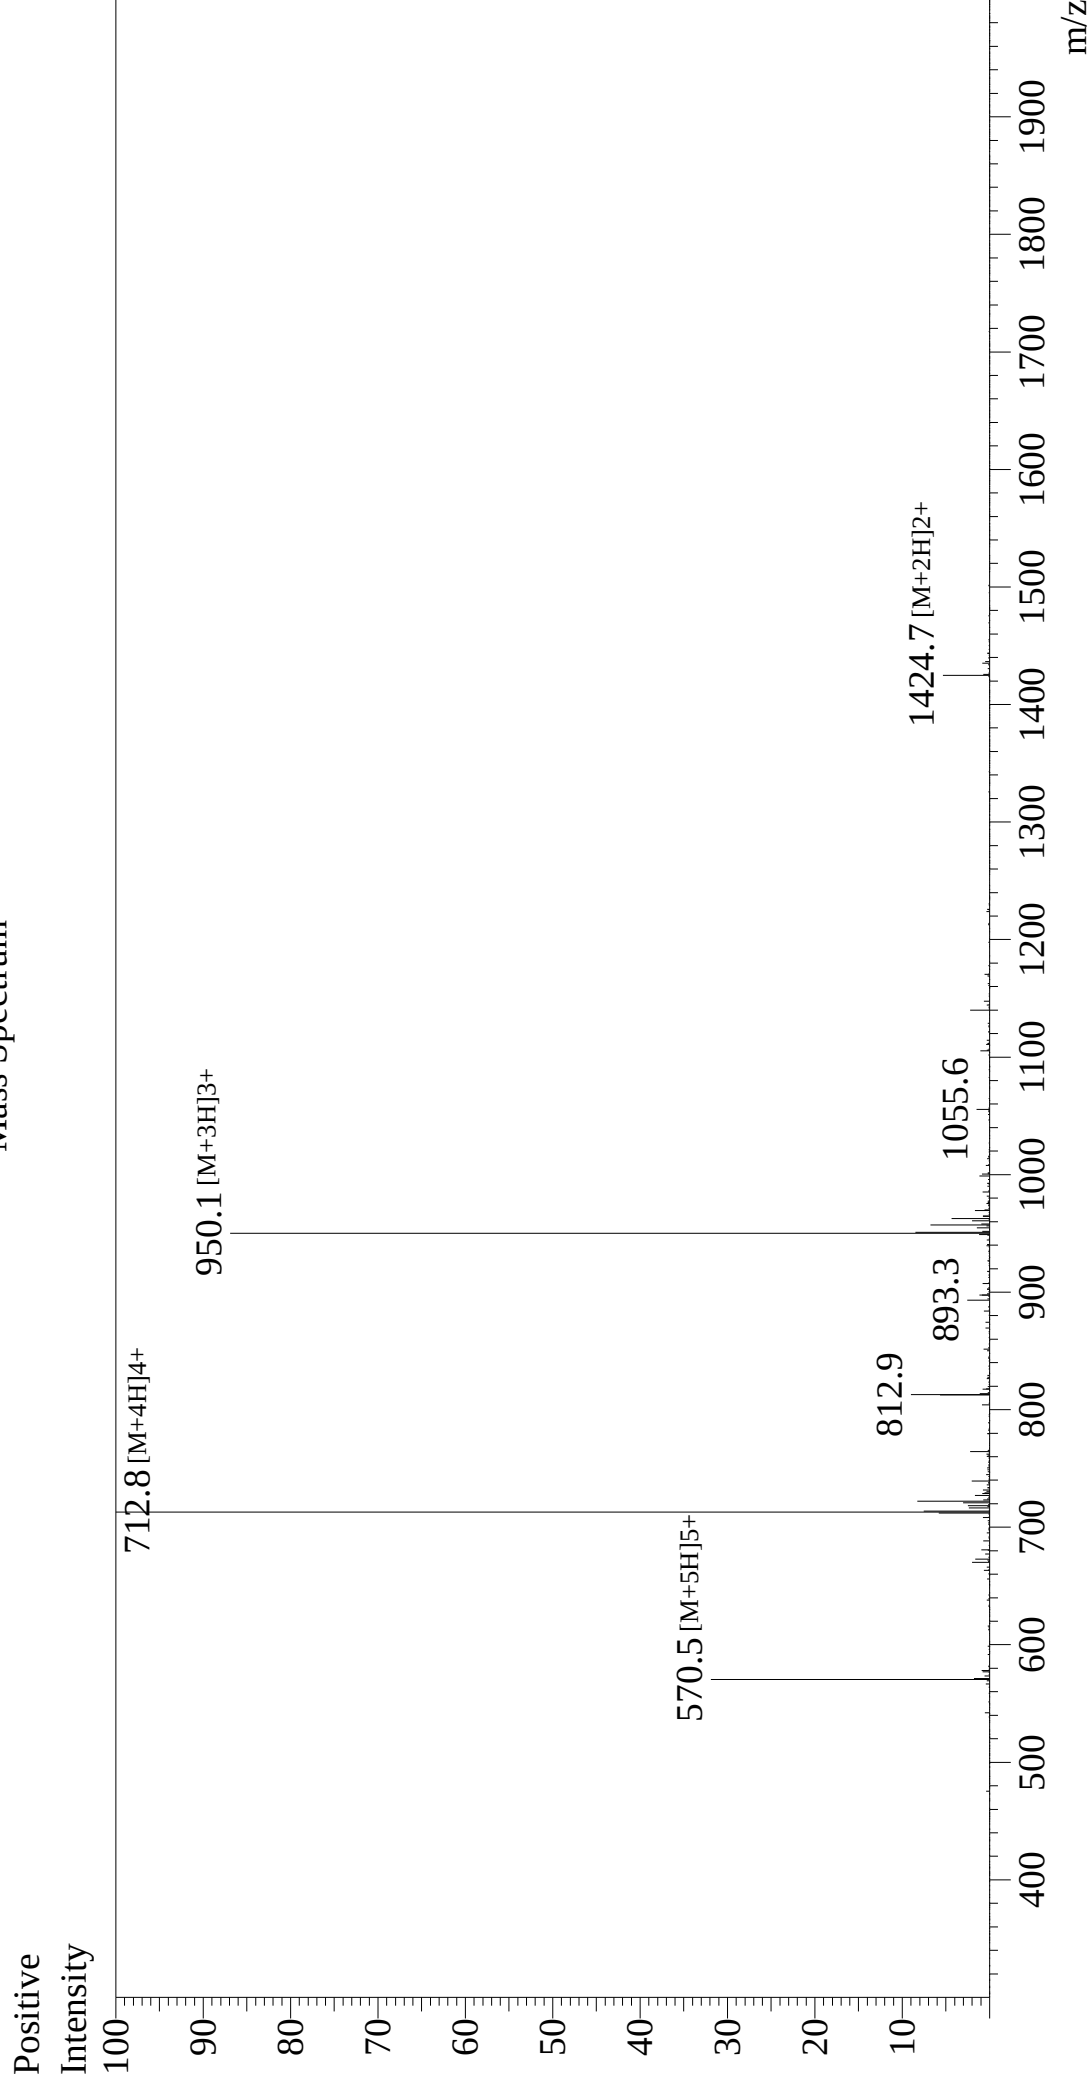

Sample Information

Month-Day Processed : 01/31/26
Time Processed : 13:20:51
Injection Volume : 0.5
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : E2548826A
Theoretical MW: 2847.50
Observed MW : 2847.2

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH