


Mass Spectrum

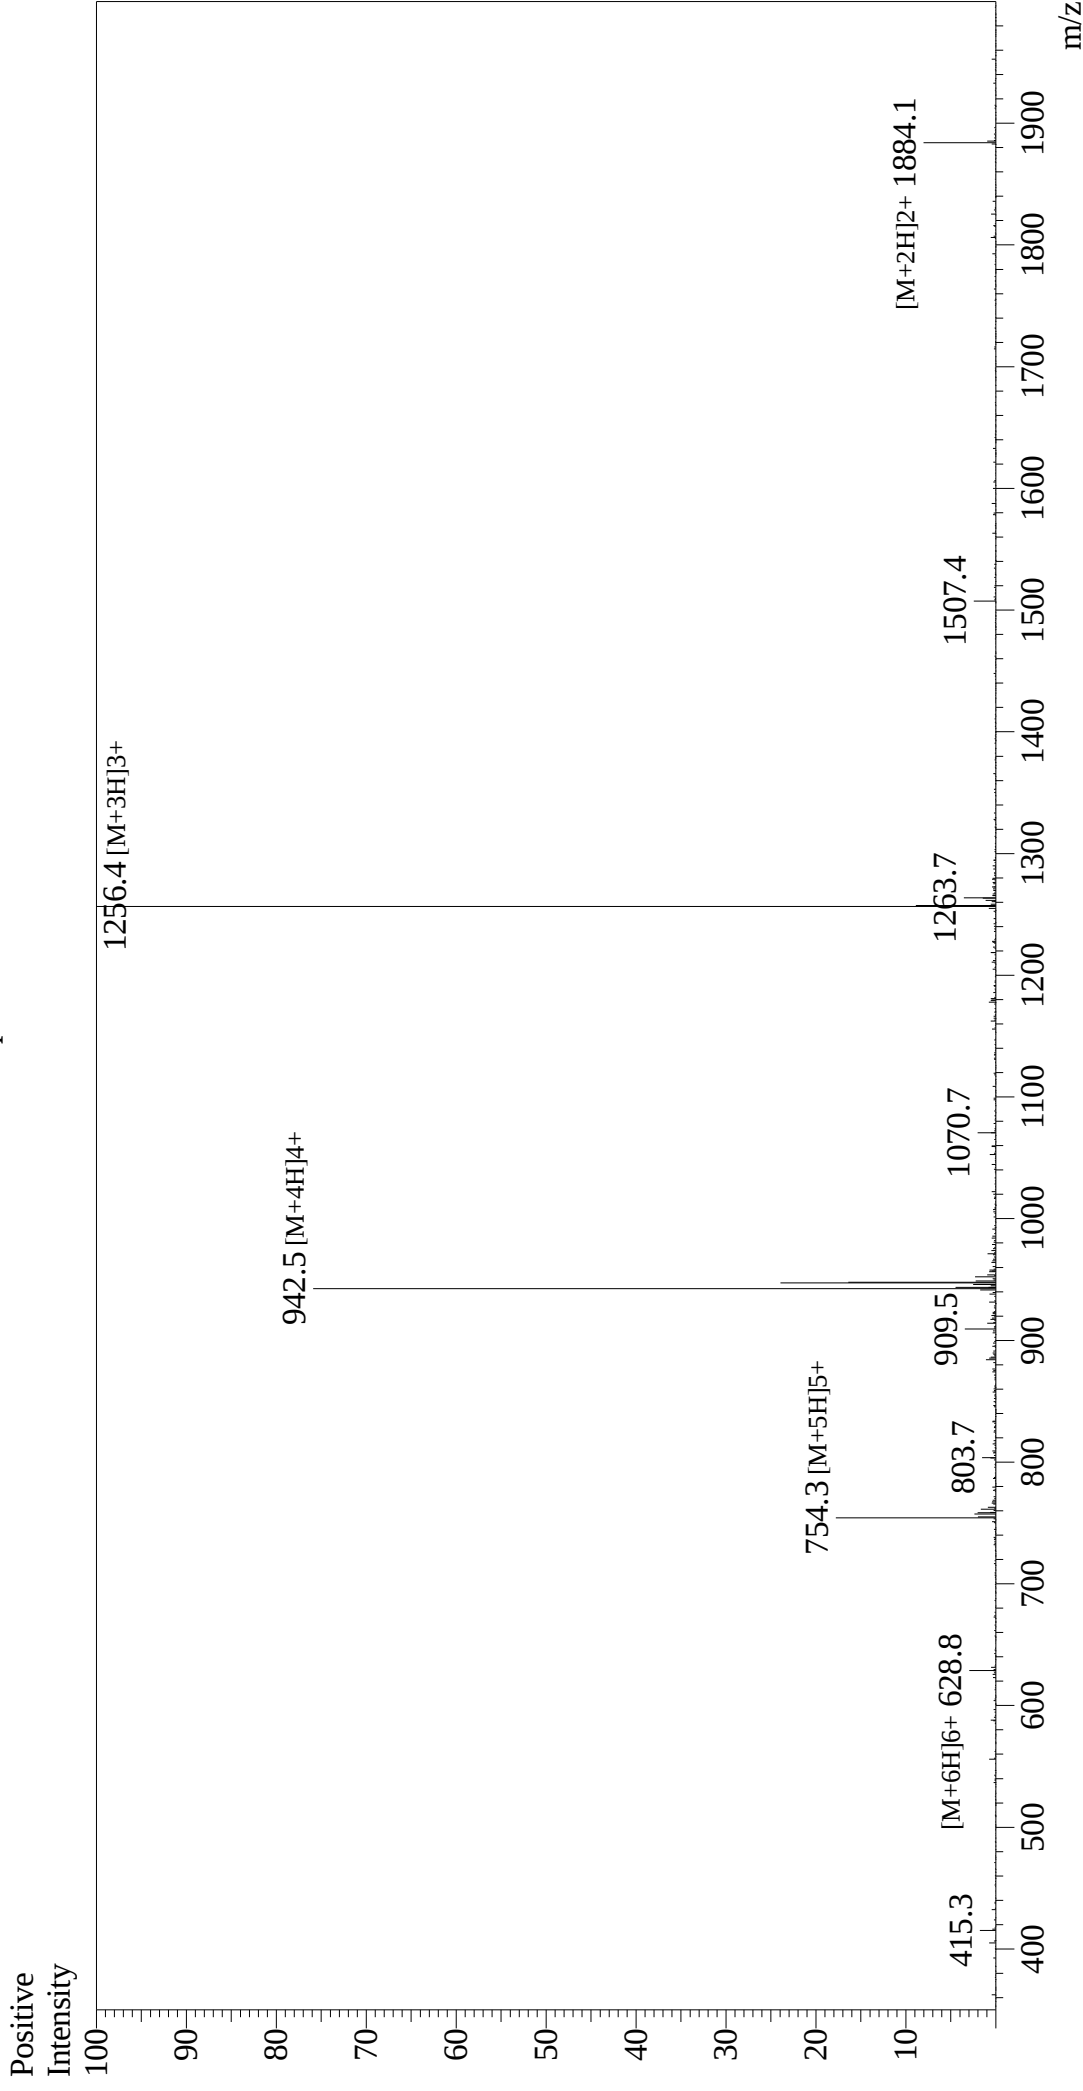

Sample Information

Month-Day Processed : 12/10/24

Time Processed : 8:49:31

Injection Volume : 0.4

Sample Name :

Cat No. : RP10769

Lot No. : E2577224L

Theoretical MW : 3766.20

Observed MW : 3766.2

Interface

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias : +4.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50%H2O/50%MeOH

Glucagon-Like Peptide (GLP) II, human