

Sample Name:β-Endorphin, human
Cat No. : RP11344
Lot No. : E2656424B
Time Processed :7:44:38 PM
Month-Day-Year Processed :03/03/2024
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ20010139

<Chromatogram>

mV

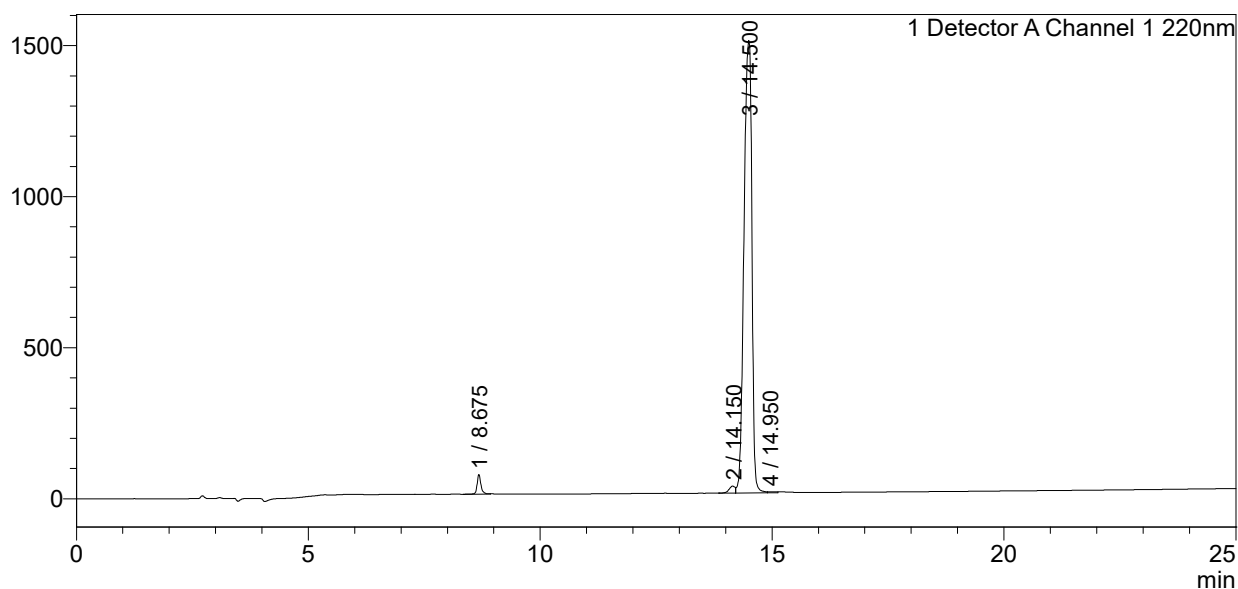

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.675	385394	64907	2.118
2	14.150	204509	22800	1.124
3	14.500	17561480	1498249	96.529
4	14.950	41642	3403	0.229
Total		18193024	1589359	100.000