

Sample Name :Substance P  
Cat No. : RP10178  
Lot No. : E3010424C  
Time Processed :10:03:55  
Month-Day-Year Processed :04/01/2024  
Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
Equipment: ZJ21010375

<Chromatogram>

mV

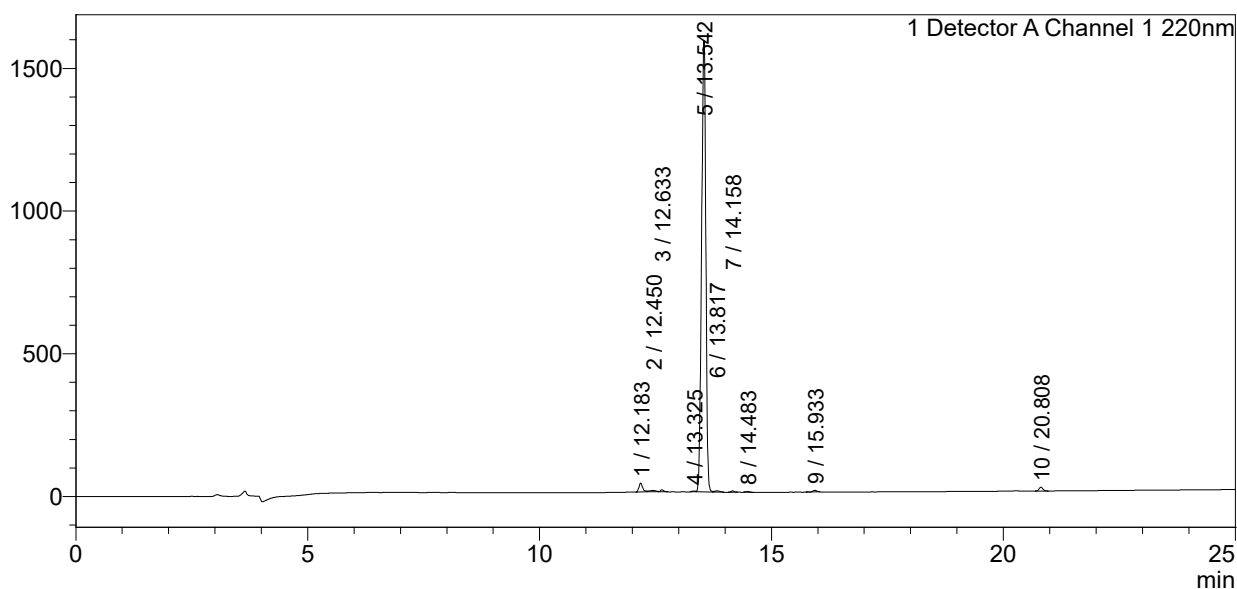

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.183	175051	30816	1.651
2	12.450	50632	4859	0.477
3	12.633	33500	7007	0.316
4	13.325	14231	2740	0.134
5	13.542	10153815	1581527	95.738
6	13.817	33386	4151	0.315
7	14.158	23006	4501	0.217
8	14.483	13870	2450	0.131
9	15.933	31618	5763	0.298
10	20.808	76771	13389	0.724
Total		10605880	1657204	100.000