

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E3100224A
 Time Processed :6:43:10
 Month-Day-Year Processed :01/20/2024
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Pumps | Solvent B Conc. | 5 |
| 33.01 | Controller | Stop | |

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ19010015

<Chromatogram>

mV

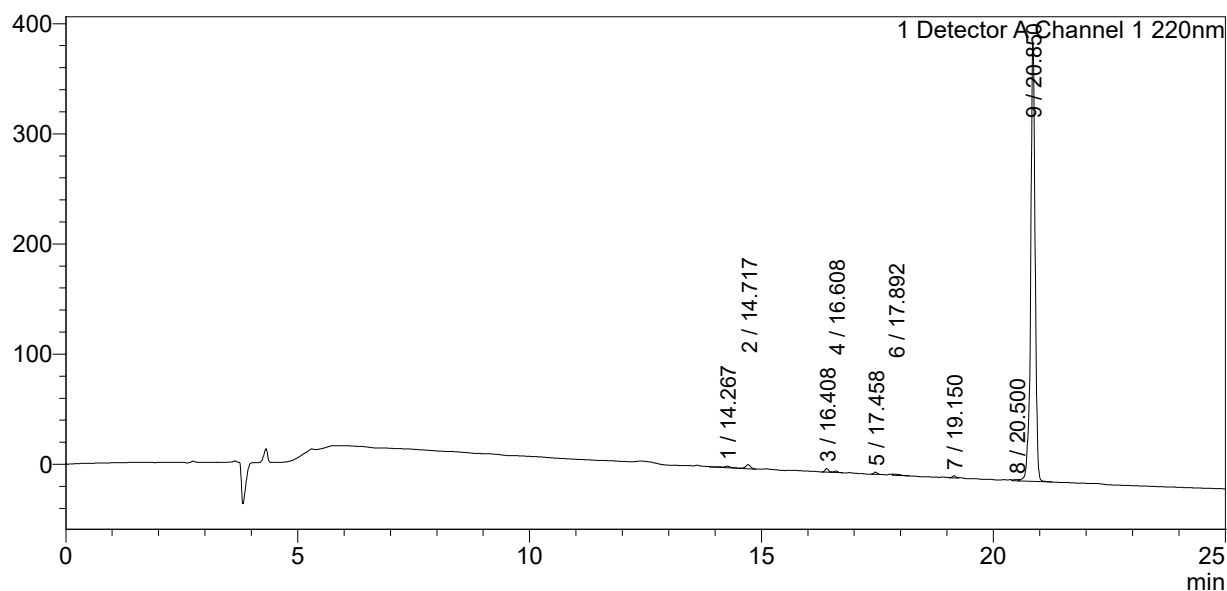

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 14.267 | 19476 | 1506 | 0.702 |
| 2 | 14.717 | 25801 | 3572 | 0.930 |
| 3 | 16.408 | 17461 | 3310 | 0.630 |
| 4 | 16.608 | 7528 | 1327 | 0.271 |
| 5 | 17.458 | 10318 | 1994 | 0.372 |
| 6 | 17.892 | 10181 | 1002 | 0.367 |
| 7 | 19.150 | 10152 | 2031 | 0.366 |
| 8 | 20.500 | 7744 | 1049 | 0.279 |
| 9 | 20.850 | 2664733 | 398338 | 96.082 |
| Total | | 2773394 | 414128 | 100.000 |