


Mass Spectrum

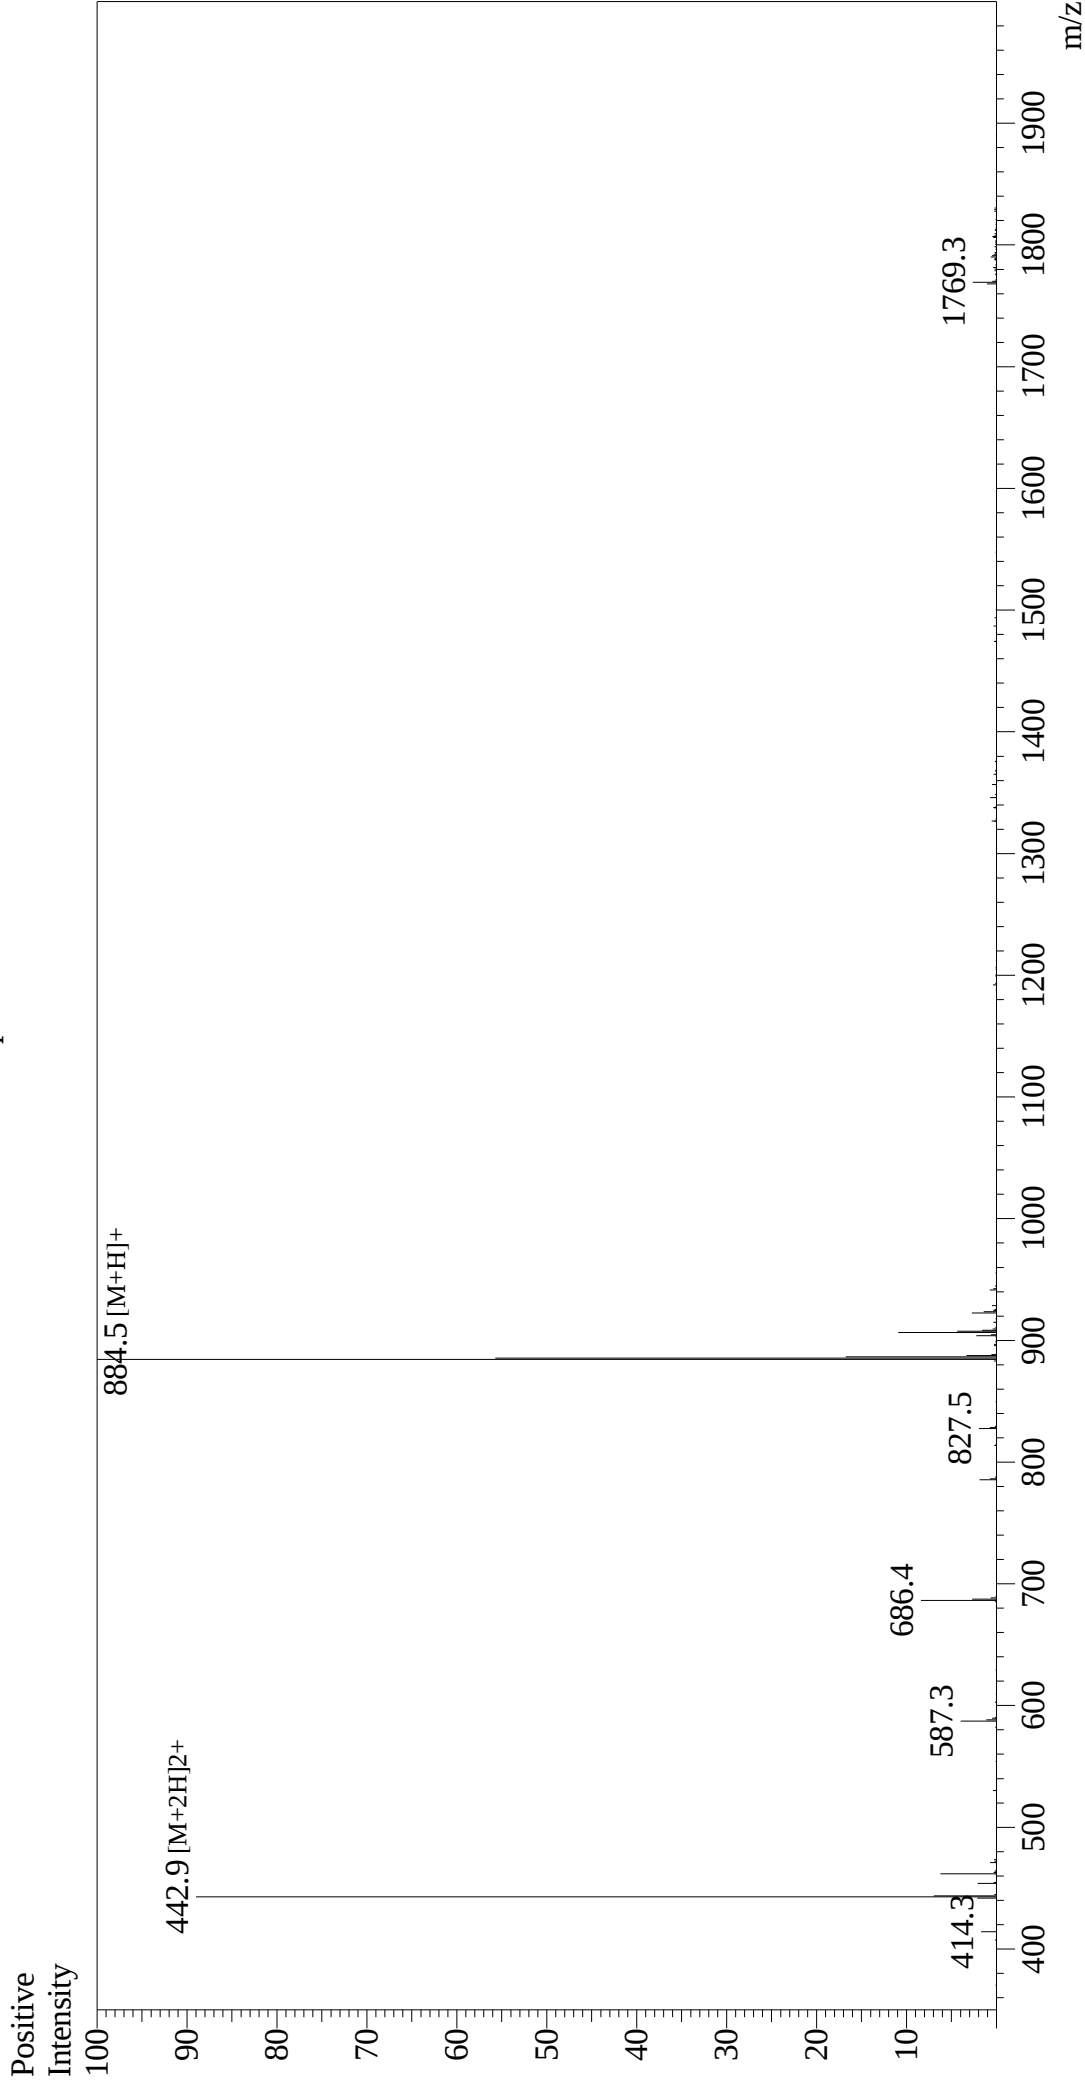

Sample Information

Month-Day Processed : 07/14/24
Time Processed : 13:04:17
Injection Volume : 0.2
Sample Name : KRAS G12V Peptide (VVVGAVGVGK)
Cat No. : RP30229
Lot No. : E3143724G
Theoretical MW : 884.08
Observed MW : 883.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH