


Sample Name :Calcitonin Gene Related Peptide (CGRP), rat  
Cat No. : RP11095  
Lot No. : E3336925D  
Time Processed :1:08:59  
Month-Day-Year Processed :05/18/2025  
Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command | Value |
|-------|------------|---------|-------|
| 0.01  | Pumps      | B.Conc  | 5     |
| 25.00 | Pumps      | B.Conc  | 65    |
| 25.01 | Pumps      | B.Conc  | 95    |
| 27.00 | Pumps      | B.Conc  | 95    |
| 27.01 | Pumps      | B.Conc  | 5     |
| 35.00 | Pumps      | B.Conc  | 5     |
| 35.01 | Controller | Stop    |       |

<<Column Performance>>  
<Detector A>  
Column :Inertsil ODS-3 4.6 x 250 mm  
Equipment: ZJ19010142

<Chromatogram>

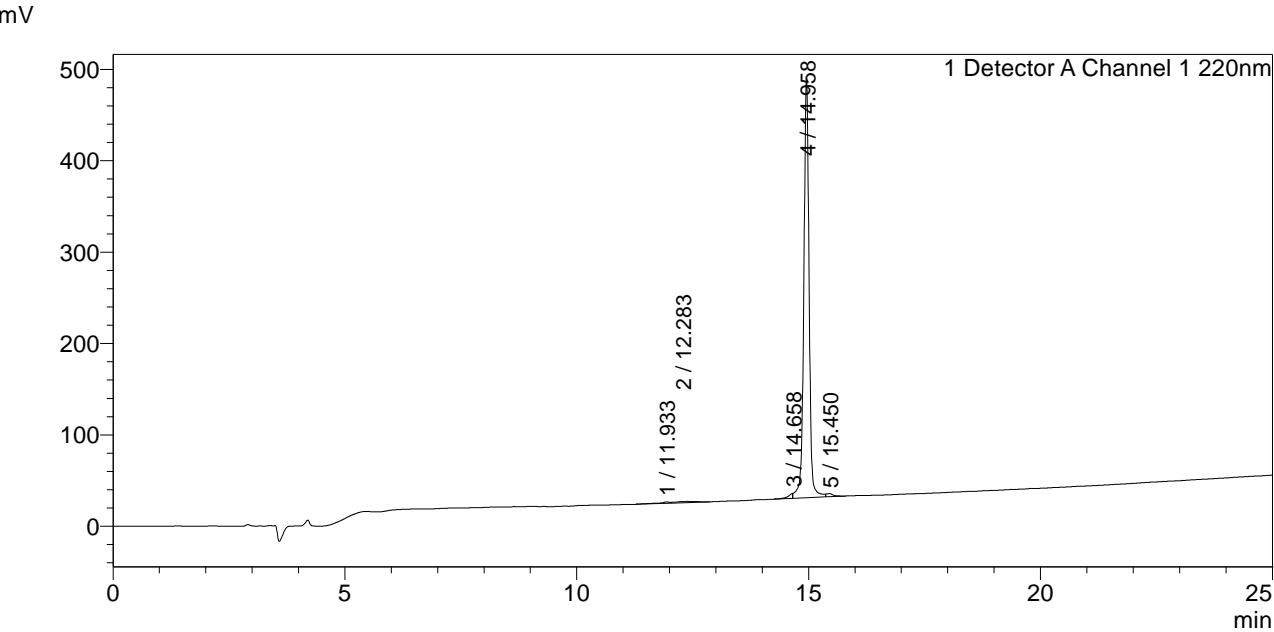

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height | Area%   |
|-------|-----------|---------|--------|---------|
| 1     | 11.933    | 23949   | 1607   | 0.635   |
| 2     | 12.283    | 39474   | 1343   | 1.047   |
| 3     | 14.658    | 36844   | 5413   | 0.977   |
| 4     | 14.958    | 3633822 | 456889 | 96.374  |
| 5     | 15.450    | 36441   | 3398   | 0.966   |
| Total |           | 3770530 | 468650 | 100.000 |